



AU9475723

(12) PATENT ABRIDGMENT (11) Document No. AU-B-75723/94
(19) AUSTRALIAN PATENT OFFICE (10) Acceptance No. 685495

- (54) Title
BLOOD COMPONENT COLLECTION SYSTEM WITH OPTIMIZER
- International Patent Classification(s)
(51)⁵ **A61M 001/00 G01N 033/49**
- (21) Application No. : **75723/94** (22) Application Date : **11.10.94**
- (30) Priority Data
- (31) Number (32) Date (33) Country
140254 21.10.93 US UNITED STATES OF AMERICA
- (43) Publication Date : **11.05.95**
- (44) Publication Date of Accepted Application : **22.01.98**
- (71) Applicant(s)
COBE LABORATORIES, INC.
- (72) Inventor(s)
ROBERT W LANGLEY; JOHN J KELLER; STEVEN GAGE URDAHL
- (74) Attorney or Agent
GRIFFITH HACK , GPO Box 1285K, MELBOURNE VIC 3001
- (56) Prior Art Documents
US 5324422
US 5178603
US 5024231
- (57) Claim

1. A method for collecting at least one predetermined type of blood component from a source of whole blood using a blood component collection system comprising a blood component collection device and collection procedure, said collection procedure having a plurality of parameters associated therewith, said method comprising the steps of:

providing biological data relating to a source of whole blood, said source being a human donor and said data comprising at least one of said donor's hematocrit, height, weight, and sex;

identifying a desired yield of at least one predetermined type of blood component;

associating a magnitude with each of a plurality of parameters associated with a collection procedure to be performed on said whole blood using a blood component collection system comprising a blood component collection device and said collection procedure, said associating step comprising performing a first deriving step comprising deriving a magnitude for at least one of said parameters from said providing and identifying steps;

(11) AU-B-75723/94
(10) 685495

-2-

inputting said magnitude of each said parameter into said blood component collection system after said associating step; and

performing said collection procedure on said blood component collection device using said inputting step to collect said desired yield of said at least on predetermined type of blood component from said source of whole blood.

685495

P/00/001
Section 29

AUSTRALIA
Patents Act 1990

PATENT REQUEST : STANDARD PATENT

I/We, being the person(s) identified below as the Applicant(s), request the grant of a Standard Patent to the person(s) identified below as the Nominated Person(s), for an invention described in the accompanying complete specification.

**Applicant(s) and
Nominated Person(s):** COBE LABORATORIES, INC.

Address: 1185 OAK STREET
LAKEWOOD, CO 80215-4407
U.S.A.

Invention Title: BLOOD COMPONENT COLLECTION SYSTEM WITH
OPTIMIZER

**Name(s) of Actual
Inventor(s):** ROBERT W LANGLEY; JOHN J KELLER;
STEVEN GAGE URDAHL

Address for Service: GRIFFITH HACK & CO
509 ST KILDA ROAD
MELBOURNE VIC 3004

Attorney Code: HA


BASIC CONVENTION APPLICATION DETAILS

Application No:	Country:	Application Date:
140254	US	21 October 1993

Drawing number recommended to accompany the abstract: 1

DATED: 11 October 1994
COBE LABORATORIES, INC.

GRIFFITH HACK & CO.



Patent Attorney for and
on behalf of the Applicant

AUSTRALIA
Patents Act 1990

NOTICE OF ENTITLEMENT

I/We COBE LABORATORIES, INC.

of 1185 OAK STREET
LAKEWOOD, CO 80215-4407
U.S.A.

being the applicant(s) in respect of an application for a patent for an invention entitled
BLOOD COMPONENT COLLECTION SYSTEM WITH OPTIMIZER, state the
following:

1. The nominated person(s) has/have, for the following reasons, gained entitlement
from the actual inventor(s):

THE NOMINATED PERSON IS THE ASSIGNEE OF
THE ACTUAL INVENTORS.

2. The nominated person(s) has/have, for the following reasons, gained entitlement
from the basic applicant(s) listed on the patent request:

THE APPLICANT AND NOMINATED PERSON IS THE
ASSIGNEE OF THE BASIC APPLICANTS.

3. The basic application(s) listed on the request form is/are the first application(s)
made in a Convention country in respect of the invention.

DATE: 11 October 1994

COBE LABORATORIES, INC.

GRIFFITH HACK & CO.



Patent Attorney for and
on behalf of the applicant(s)

AUSTRALIA
Patents Act 1990

COMPLETE SPECIFICATION
STANDARD PATENT

Applicant(s):

COBE LABORATORIES, INC.

Invention Title:

BLOOD COMPONENT COLLECTION SYSTEM WITH
OPTIMIZER

The following statement is a full description of this
invention, including the best method of performing it known
to me/us:

BLOOD COMPONENT SYSTEM
WITH OPTIMIZER

Field of the Invention

- 5 The present invention generally relates to the field of blood component collection systems and, more particularly, to providing management capabilities by incorporating optimization principles into such systems.

10 Background of the Invention

- The utilization of blood taken from donors and infused into recipients is well known for purposes of treating medical emergencies and other conditions. More recently, selected blood components have been separated and
15 collected from blood for subsequent infusion into recipients requiring blood component therapy. The primary blood components include platelets, red blood cells, white blood cells, and plasma.

2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
61
62
63
64
65
66
67
68
69
70
71
72
73
74
75
76
77
78
79
80
81
82
83
84
85
86
87
88
89
90
91
92
93
94
95
96
97
98
99
100
101
102
103
104
105
106
107
108
109
110
111
112
113
114
115
116
117
118
119
120
121
122
123
124
125
126
127
128
129
130
131
132
133
134
135
136
137
138
139
140
141
142
143
144
145
146
147
148
149
150
151
152
153
154
155
156
157
158
159
160
161
162
163
164
165
166
167
168
169
170
171
172
173
174
175
176
177
178
179
180
181
182
183
184
185
186
187
188
189
190
191
192
193
194
195
196
197
198
199
200
201
202
203
204
205
206
207
208
209
210
211
212
213
214
215
216
217
218
219
220
221
222
223
224
225
226
227
228
229
230
231
232
233
234
235
236
237
238
239
240
241
242
243
244
245
246
247
248
249
250
251
252
253
254
255
256
257
258
259
260
261
262
263
264
265
266
267
268
269
270
271
272
273
274
275
276
277
278
279
280
281
282
283
284
285
286
287
288
289
290
291
292
293
294
295
296
297
298
299
300
301
302
303
304
305
306
307
308
309
310
311
312
313
314
315
316
317
318
319
320
321
322
323
324
325
326
327
328
329
330
331
332
333
334
335
336
337
338
339
340
341
342
343
344
345
346
347
348
349
350
351
352
353
354
355
356
357
358
359
360
361
362
363
364
365
366
367
368
369
370
371
372
373
374
375
376
377
378
379
380
381
382
383
384
385
386
387
388
389
390
391
392
393
394
395
396
397
398
399
400
401
402
403
404
405
406
407
408
409
410
411
412
413
414
415
416
417
418
419
420
421
422
423
424
425
426
427
428
429
430
431
432
433
434
435
436
437
438
439
440
441
442
443
444
445
446
447
448
449
450
451
452
453
454
455
456
457
458
459
460
461
462
463
464
465
466
467
468
469
470
471
472
473
474
475
476
477
478
479
480
481
482
483
484
485
486
487
488
489
490
491
492
493
494
495
496
497
498
499
500
501
502
503
504
505
506
507
508
509
510
511
512
513
514
515
516
517
518
519
520
521
522
523
524
525
526
527
528
529
530
531
532
533
534
535
536
537
538
539
540
541
542
543
544
545
546
547
548
549
550
551
552
553
554
555
556
557
558
559
560
561
562
563
564
565
566
567
568
569
570
571
572
573
574
575
576
577
578
579
580
581
582
583
584
585
586
587
588
589
590
591
592
593
594
595
596
597
598
599
600
601
602
603
604
605
606
607
608
609
610
611
612
613
614
615
616
617
618
619
620
621
622
623
624
625
626
627
628
629
630
631
632
633
634
635
636
637
638
639
640
641
642
643
644
645
646
647
648
649
650
651
652
653
654
655
656
657
658
659
660
661
662
663
664
665
666
667
668
669
670
671
672
673
674
675
676
677
678
679
680
681
682
683
684
685
686
687
688
689
690
691
692
693
694
695
696
697
698
699
700
701
702
703
704
705
706
707
708
709
710
711
712
713
714
715
716
717
718
719
720
721
722
723
724
725
726
727
728
729
730
731
732
733
734
735
736
737
738
739
740
741
742
743
744
745
746
747
748
749
750
751
752
753
754
755
756
757
758
759
760
761
762
763
764
765
766
767
768
769
770
771
772
773
774
775
776
777
778
779
780
781
782
783
784
785
786
787
788
789
790
791
792
793
794
795
796
797
798
799
800
801
802
803
804
805
806
807
808
809
810
811
812
813
814
815
816
817
818
819
820
821
822
823
824
825
826
827
828
829
830
831
832
833
834
835
836
837
838
839
840
841
842
843
844
845
846
847
848
849
850
851
852
853
854
855
856
857
858
859
860
861
862
863
864
865
866
867
868
869
870
871
872
873
874
875
876
877
878
879
880
881
882
883
884
885
886
887
888
889
890
891
892
893
894
895
896
897
898
899
900
901
902
903
904
905
906
907
908
909
910
911
912
913
914
915
916
917
918
919
920
921
922
923
924
925
926
927
928
929
930
931
932
933
934
935
936
937
938
939
940
941
942
943
944
945
946
947
948
949
950
951
952
953
954
955
956
957
958
959
960
961
962
963
964
965
966
967
968
969
970
971
972
973
974
975
976
977
978
979
980
981
982
983
984
985
986
987
988
989
990
991
992
993
994
995
996
997
998
999
1000
1001
1002
1003
1004
1005
1006
1007
1008
1009
1010
1011
1012
1013
1014
1015
1016
1017
1018
1019
1020
1021
1022
1023
1024
1025
1026
1027
1028
1029
1030
1031
1032
1033
1034
1035
1036
1037
1038
1039
1040
1041
1042
1043
1044
1045
1046
1047
1048
1049
1050
1051
1052
1053
1054
1055
1056
1057
1058
1059
1060
1061
1062
1063
1064
1065
1066
1067
1068
1069
1070
1071
1072
1073
1074
1075
1076
1077
1078
1079
1080
1081
1082
1083
1084
1085
1086
1087
1088
1089
1090
1091
1092
1093
1094
1095
1096
1097
1098
1099
1100
1101
1102
1103
1104
1105
1106
1107
1108
1109
1110
1111
1112
1113
1114
1115
1116
1117
1118
1119
1120
1121
1122
1123
1124
1125
1126
1127
1128
1129
1130
1131
1132
1133
1134
1135
1136
1137
1138
1139
1140
1141
1142
1143
1144
1145
1146
1147
1148
1149
1150
1151
1152
1153
1154
1155
1156
1157
1158
1159
1160
1161
1162
1163
1164
1165
1166
1167
1168
1169
1170
1171
1172
1173
1174
1175
1176
1177
1178
1179
1180
1181
1182
1183
1184
1185
1186
1187
1188
1189
1190
1191
1192
1193
1194
1195
1196
1197
1198
1199
1200
1201
1202
1203
1204
1205
1206
1207
1208
1209
1210
1211
1212
1213
1214
1215
1216
1217
1218
1219
1220
1221
1222
1223
1224
1225
1226
1227
1228
1229
1230
1231
1232
1233
1234
1235
1236
1237
1238
1239
1240
1241
1242
1243
1244
1245
1246
1247
1248
1249
1250
1251
1252
1253
1254
1255
1256
1257
1258
1259
1260
1261
1262
1263
1264
1265
1266
1267
1268
1269
1270
1271
1272
1273
1274
1275
1276
1277
1278
1279
1280
1281
1282
1283
1284
1285
1286
1287
1288
1289
1290
1291
1292
1293
1294
1295
1296
1297
1298
1299
1300
1301
1302
1303
1304
1305
1306
1307
1308
1309
1310
1311
1312
1313
1314
1315
1316
1317
1318
1319
1320
1321
1322
1323
1324
1325
1326
1327
1328
1329
1330
1331
1332
1333
1334
1335
1336
1337
1338
1339
1340
1341
1342
1343
1344
1345
1346
1347
1348
1349
1350
1351
1352
1353
1354
1355
1356
1357
1358
1359
1360
1361
1362
1363
1364
1365
1366
1367
1368
1369
1370
1371
1372
1373
1374
1375
1376
1377
1378
1379
1380
1381
1382
1383
1384
1385
1386
1387
1388
1389
1390
1391
1392
1393
1394
1395
1396
1397
1398
1399
1400
1401
1402
1403
1404
1405
1406
1407
1408
1409
1410
1411
1412
1413
1414
1415
1416
1417
1418
1419
1420
1421
1422
1423
1424
1425
1426
1427
1428
1429
1430
1431
1432
1433
1434
1435
1436
1437
1438
1439
1440
1441
1442
1443
1444
1445
1446
1447
1448
1449
1450
1451
1452
1453
1454
1455
1456
1457
1458
1459
1460
1461
1462
1463
1464
1465
1466
1467
1468
1469
1470
1471
1472
1473
1474
1475
1476
1477
1478
1479
1480
1481
1482
1483
1484
1485
1486
1487
1488
1489
1490
1491
1492
1493
1494
1495
1496
1497
1498
1499
1500
1501
1502
1503
1504
1505
1506
1507
1508
1509
1510
1511
1512
1513
1514
1515
1516
1517
1518
1519
1520
1521
1522
1523
1524
1525
1526
1527
1528
1529
1530
1531
1532
1533
1534
1535
1536
1537
1538
1539
1540
1541
1542
1543
1544
1545
1546
1547
1548
1549
1550
1551
1552
1553
1554
1555
1556
1557
1558
1559
1560
1561
1562
1563
1564
1565
1566
1567
1568
1569
1570
1571
1572
1573
1574
1575
1576
1577
1578
1579
1580
1581
1582
1583
1584
1585
1586
1587
1588
1589
1590
1591
1592
1593
1594
1595
1596
1597
1598
1599
1600
1601
1602
1603
1604
1605
1606
1607
1608
1609
1610
1611
1612
1613
1614
1615
1616
1617
1618
1619
1620
1621
1622
1623
1624
1625
1626
1627
1628
1629
1630
1631
1632
1633
1634
1635
1636
1637
1638
1639
1640
1641
1642
1643
1644
1645
1646
1647
1648
1649
1650
1651
1652
1653
1654
1655
1656
1657
1658
1659
1660
1661
1662
1663
1664
1665
1666
1667
1668
1669
1670
1671
1672
1673
1674
1675
1676
1677
1678
1679
1680
1681
1682
1683
1684
1685
1686
1687
1688
1689
1690
1691
1692
1693
1694
1695
1696
1697
1698
1699
1700
1701
1702
1703
1704
1705
1706
1707
1708
1709
1710
1711
1712
1713
1714
1715
1716
1717
1718
1719
1720
1721
1722
1723
1724
1725
1726
1727
1728
1729
1730
1731
1732
1733
1734
1735
1736
1737
1738
1739
1740
1741
1742
1743
1744
1745
1746
1747
1748
1749
1750
1751
1752
1753
1754
1755
1756
1757
1758
1759
1760
1761
1762
1763
1764
1765
1766
1767
1768
1769
1770
1771
1772
1773
1774
1775
1776
1777
1778
1779
1780
1781
1782
1783
1784
1785
1786
1787
1788
1789
1790
1791
1792
1793
1794
1795
1796
1797
1798
1799
1800
1801
1802
1803
1804
1805
1806
1807
1808
1809
1810
1811
1812
1813
1814
1815
1816
1817
1818
1819
1820
1821
1822
1823
1824
1825
1826
1827
1828
1829
1830
1831
1832
1833
1834
1835
1836
1837
1838
1839
1840
1841
1842
1843
1844
1845
1846
1847
1848
1849
1850
1851
1852
1853
1854
1855
1856
1857
1858
1859
1860
1861
1862
1863
1864
1865
1866
1867
1868
1869
1870
1871
1872
1873
1874
1875
1876
1877
1878
1879
1880
1881
1882
1883
1884
1885
1886
1887
1888
1889
1890
1891
1892
1893
1894
1895
1896
1897
1898
1899
1900
1901
1902
1903
1904
1905
1906
1907
1908
1909
1910
1911
1912
1913
1914
1915
1916
1917
1918
1919
1920
1921
1922
1923
1924
1925
1926
1927
1928
1929
1930
1931
1932
1933
1934
1935
1936
1937
1938
1939
1940
1941
1942
1943
1944
1945
1946
1947
1948
1949
1950
1951
1952
1953
1954
1955
1956
1957
1958
1959
1960
1961
1962
1963
1964
1965
1966
1967
1968
1969
1970
1971
1972
1973
1974
1975
1976
1977
1978
1979
1980
1981
1982
1983
1984
1985
1986
1987
1988
1989
1990
1991
1992
1993
1994
1995
1996
1997
1998
1999
2000
2001
2002
2003
2004
2005
2006
2007
2008
2009
2010
2011
2012
2013
2014
2015
2016
2017
2018
2019
2020
2021
2022
2023
2024
2025
2026
2027
2028
2029
2030
2031
2032
2033
2034
2035
2036
2037
2038
2039
2040
2041
2042
2043
2044
2045
2046
2047
2048
2049
2050
2051
2052
2053
2054
2055
2056
2057
2058
2059
2060
2061
2062
2063
2064
2065
2066
2067
2068
2069
2070
2071
2072
2073
2074
2075
2076
2077
2078
2079
2080
2081
2082
2083
2084
2085
2086
2087
2088
2089
2090
2091
2092
2093
2094
2095
2096
2097
2098
2099
2100
2101
2102
2103
2104
2105
2106
2107
2108
2109
2110
2111
2112
2113
2114
2115
2116
2117
2118
2119
2120
2121
2122
2123
2124
2125
2126
2127
2128
2129
2130
2131
2132
2133
2134
2135
2136
2137
2138
2139
2140
2141
2142
2143
2144
2145
2146
2147
2148
2149
2150
2151
2152
2153
2154
2155
2156
2157
2158
2159
2160
2161
2162
2163
2164
2165
2166
2167
2168
2169
2170
2171
2172
2173
2174
2175
2176
2177
2178
2179
2180
2181
2182
2183
2184
2185
2186
218

In order to collect blood components, blood is removed from a donor by a needle assembly or other blood access device and is thereafter processed utilizing centrifugation or other appropriate separation techniques to isolate and collect the desired components. This procedure is carried out most effectively in an on-line process wherein blood is removed from a donor, processed through a disposable extracorporeal circuit to obtain the desired components, and thereafter returned to the donor. One blood component collection system which provides for this type of blood component collection procedure is the COBE Spectra™ which is commercially available from the assignee of the present application.

The yield of a particular collection of blood components is an important factor. For instance, presently in the United States a yield must be associated with a collection of blood components in order to be a useful blood component product. COBE Spectra™ presently accommodates for this requirement by processing certain donor biological data such as height, weight, sex, and hematocrit, preconfigured/operator-input data such as the total procedure time, and system-related data such as the type of collection procedure (e.g., single or double needle) and collection efficiency to generate certain process parameters such as the inlet flow to COBE Spectra™ (a combined flow of whole blood from the donor plus typically a flow of anticoagulant) and a predicted blood component yield as well.

An additional consideration presently in the United States relating to blood component yield is that it is determinative of the product classification. With regard to platelets, presently a single platelet product is considered to be a collection of 3×10^{11} platelets and a double platelet product is considered to be a collection of 6×10^{11} platelets. If the collection is between 3×10^{11} and 6×10^{11} platelets it is still considered to be a single platelet product. This classification as a single or double platelet product is relevant to blood component collection facilities (e.g., blood banks/centers) since a double platelet product has a higher selling price associated therewith than a single platelet product and also typically benefits more patients. The yield of a particular collection of blood components may also be a relevant consideration for certain therapeutic treatments.

Other important considerations relating to blood component collection systems relate to the donor. For instance, blood component collection facilities are not only experiencing an increase in the overall demand for blood components, but the demand now typically varies between the blood component types as well. Moreover, not only is the supply of donors unfortunately in many cases inadequate, but donor time constraints are becoming more prevalent. Furthermore, obtainable yields from a given donor may vary from one blood component to another (i.e., one donor may be a better platelet source than a red blood cell source).

Based upon the foregoing, the management of the various aspects of blood component collection systems is becoming increasingly important.

5 Summary of the Invention

According to a first aspect of the present invention there is provided a method for collecting at least one predetermined type of blood component from a source of whole blood using a blood component collection
10 system comprising a blood component collection device and collection procedure, said collection procedure having a plurality of parameters associated therewith, said method comprising the steps of:

providing biological data relating to a source of
15 whole blood, said source being a human donor and said data comprising at least one of said donor's hematocrit, height, weight, and sex;

identifying a desired yield of at least one predetermined type of blood component;

20 associating a magnitude with each of a plurality of parameters associated with a collection procedure to be performed on said whole blood using a blood component collection system comprising a blood component collection device and said collection procedure, said associating step
25 comprising performing a first deriving step comprising deriving a magnitude for at least one of said parameters from said providing and identifying steps;

inputting said magnitude of each said parameter into said blood component collection system after said
30 associating step; and

performing said collection procedure on said blood component collection device using said inputting step to collect said desired yield of said at least one predetermined type of blood component from said source of
35 whole blood.

According to a second aspect of the present invention there is also provided a method for collecting a



blood component from a source of whole blood using a blood component collection system comprising a blood component collection device and collection procedure, wherein an inlet flow to said blood component collection system
5 comprises a flow of whole blood from said source and a flow of anticoagulant, said method comprising the steps of:

identifying a total procedure time for a collection procedure to be performed on a source of whole blood to obtain a plurality of at least one type of blood component therefrom using a blood component collection
10 system comprising a blood component collection device and said collection procedure;

deriving a first inlet flow to said collection system which provides a maximum yield of said blood
15 components;

deriving a second inlet flow to said collection system using at least said identifying a total procedure time step;

identifying a smallest magnitude of said first and second inlet flow as an actual inlet flow to said blood component collection system; and
20

performing said collection procedure with said blood component collection device, using said actual inlet flow, and for said total procedure time to collect said
25 blood components from said source of whole blood.

According to a third aspect of the present invention there is further provided a method for collecting a blood component from a donor using a blood component collection system comprising a blood component collection
30 procedure and a collection procedure, said collection device comprising a plurality of parameters, said method comprising the steps of:

providing biological data relating to a donor;
associating a magnitude with a plurality of
35 control parameters associated with a collection procedure to be performed on blood from said donor to obtain a plurality of at least one type of blood component therefrom



using a blood component collection system, said blood component collection system comprising a blood component collection device and said collection procedure, said associating step being based upon at least said providing step;

5
10
15
20
25
30
35
optimizing said magnitude of at least one or said control parameters in relation to both donor constraints and system constraints, said optimizing step allowing for achieving at least one of first and second conditions, said first condition being collecting a predetermined quantity of said blood components in a minimum amount of time and said second condition being collecting a maximum quantity of said blood components in a predetermined amount of time;

inputting said magnitudes of said parameters into said blood component collection device after said optimizing step; and

performing said collection procedure on said blood component collection device using said parameters to collect said blood components from said donor to achieve at least one of said first and second conditions.

According to a fourth aspect of the present invention there is further provided a blood component collection control and information communication system used in conjunction with a blood component collection device in a procedure performed on a donor to separate, remove and collect components from blood received from the donor, comprising:

an information communication medium;
a first station interactive with the communication medium to transmit and receive information on the medium describing biological data of the donor, describing process parameters for controlling the collection device during the procedure performed on the donor, describing physical and medical characteristics of the donor observed during performance of a prior procedure on the donor, and describing the yield of at least one component obtained from the donor during performance of the



procedure; the first station including an information input device by which to supply donor data, process parameters, prior procedure characteristics and component yield information to communication medium; the first station

5 further including a computer responsive to the donor data, prior procedure characteristics and component yield information received from the communication medium to determine at least one process parameter to be used for controlling the blood component collection device during

10 performance of a subsequent procedure on the donor; and the first station also including a display by which to display the donor data, process parameters, prior procedure characteristics and component yield information;

a second station interactive with the

15 communication medium to transmit and receive information on the medium describing biological data of the donor, describing process parameters for controlling the collection device during the procedure performed on the donor, describing physical and medical characteristics of

20 the donor observed during performance of a prior procedure on the donor, and describing the yield of at least one component obtained from the donor during performance of a procedure; the second station including an information input device by which to supply donor data, process

25 parameters, prior procedure characteristics and component yield information to communication medium; the second station further including a computer responsive to the donor data, prior procedure characteristics and component yield information received from the communication medium to

30 determine at least one process parameter to be used for controlling the blood component collection device during performance of a subsequent procedure on the donor; and the second station also including a display by which to display the donor data, process parameters, prior procedure

35 characteristics and component yield information; and

an interface of at least one of the first or second stations which connects to the blood component



collection device to the one station, the interface adaptable for controlling the blood collection device to perform the procedure in response to the process parameter information transmitted to the one station by the communication medium; the interface further supplying information to the medium at the one station describing the yield of at least one component obtained from the donor during performance of the procedure performed.

5

communication medium; the interface further supplying information to the medium at the one station describing the yield of at least one component obtained from the donor during performance of the procedure performed.

13 12 11 10 9 8 7 6 5 4 3 2 1



7

The subject invention provides greater efficiency in blood component collection and management. For example, the present invention can be used to compare blood bank/center component inventories with projected needs, and
5 adjust collection procedures to meet these needs. Further, the present invention provides benefits to donors. In particular, certain information relating to the donor's physical and medical characteristics may be stored in the system and utilized during subsequent visits by the donor
10 to derive magnitudes for the various process control parameters. For example, for a donor with an anticoagulant intolerance, the magnitude of the anticoagulant infusion rate may be set so as to not exceed the donor's tolerance.

15 Brief Description of the Drawings

Fig. 1 is a schematic representation of a blood component collection system in accordance with principles of the present invention;

Fig. 2 is a schematic representation of one embodiment
20 of a blood component separation assembly which utilizes a dual needle configuration and which may be incorporated into the blood component collection system of Fig. 1;

Fig. 3 is a schematic representation of one embodiment
25 of a blood component separation assembly which utilizes a single needle configuration and which may be incorporated into the blood component collection system of Fig. 1;

Figs. 4a and 4b are perspective and top views, respectively, of one type of a disposable processing channel used in the blood component collection device of Figs. 2 and 3;

5 Fig. 5 is a flow chart of a blood component collection procedure utilizing principles of the present invention;

Fig. 6 is a flow chart of one optimization model for deriving at least one optimal process parameter from a desired blood component yield or from a total procedure
10 time in accordance with principles of the present invention;

Fig. 7 is a flow chart of one optimization model for deriving at least one optimal process parameter from a desired blood component yield or from a total procedure
15 time in accordance with principles of the present invention; and

Fig. 8 is a yield/inlet flow curve.

Detailed Description

20 The present invention will be described with reference to the accompanying drawings which assist in illustrating the pertinent features thereof. One application of the present invention is embodied within a blood component collection system which separates, removes, and collects at
25 least one type of blood component (e.g., platelets, red blood cells, white blood cells, plasma) from a source of whole blood (e.g., a donor) through utilization of a collection procedure derived from a typically site-

7

configured/operator-input goal(s) and the "maximization" of at least one process control parameter. This type of derivation is referred to herein as an "optimization process" and the derived process control parameters are referred to herein as "optimal values."

Referring to Fig. 1, the present invention is embodied within the blood component collection system 2 which would typically be implemented at a blood bank/center (not shown). The system 2 includes an optimization assembly 140 (e.g., appropriate microprocessor(s) such as an IBM compatible PC and software) and at least one blood component collection assembly 10 (three shown) which each includes a blood component collection device 18 as an integral part thereof. As will be discussed below, the optimization assembly 140 (or at least a portion thereof) and associated blood component collection assemblies 10 are preferably appropriately interfaced but may be completely separate as well. That is, optimization procedures in accordance with principles of the present invention are not limited to being performed at any particular location.

Generally, the optimization assembly 140 includes a central input station 148 (e.g., an appropriate microprocessor such as an IBM compatible PC and attendant software) for inputting and maintaining donor-related data, and also typically for preparing an initial procedure order (the process control parameters derived from the donor-related data and other considerations) for a given donor. These procedures may also be performed at the appropriate

operator interface module 16 as well such that a central input station 148 is not required. However, where a central input station 148 is used, this donor-related data and/or initial procedure order is transferred to one of the operator interface modules 16 (e.g., an appropriate microprocessor such as an IBM compatible microprocessor and interfaced with the device 18 via an RS232 or other lab specific interface, including the Digital Equipment Corp. PCP 30, which is also known as the DEC pc 325SL and which utilizes a 386 processor) which are located at each blood component collection device 18 and which as noted preferably interfaces with an optimizer module 144 (part of the optimizing assembly 140) for providing the operator with one or more optimization options. These optimization options provide a different set of process control parameters than the initial procedure order based upon one or more specified conditions/goals (e.g., input blood component yield, input procedure time) and a particular derivation for the process control parameters. If an optimization option is selected the procedure order is modified to reflect the results of the optimization, the collection procedure is initialized/reinitialized (i.e., the collection procedure would be reinitialized in the case of an optimization which is performed after the collection procedure has been initiated and such is referenced to as a downstream optimization) with the results of the optimization, and the collection procedure is thereafter performed with the blood component collection device 18.

Various embodiments of blood component collection assemblies may incorporate principles of the present invention. However, as noted above on-line techniques have been determined to be quite effective and thus the present invention is being described with reference to such techniques. One embodiment of an on-line technique and attendant apparatus which may be incorporated into the blood component collection system 2 of Fig. 1 is illustrated in Fig. 2. The blood component collection assembly 10' utilizes an on-line technique in that a donor 14 (e.g., the whole blood source) is directly integrated with the system 10' by fluid interconnection with the blood component collection device 18. This particular on-line configuration since there are two fluid interconnections between the donor 14 and the blood component collection device 18.

20

25

30

35

The donor 14 is fluidly connected to the blood component collection device 18 by an inlet line 22 and appropriate needle assembly (not shown). Whole blood from the donor 14 is thus continuously provided to the blood component collection device 18 through the inlet line 22 for separation of the desired blood component(s) therefrom, utilizing an inlet pump 26 (e.g., a peristaltic pump) to maintain this flow if desired/required. Prior to the blood of the donor 14 entering the blood component collection device 18, anticoagulant from an anticoagulant ("AC") container 30 may be provided to the whole blood, utilizing

an AC pump 32 (e.g., a peristaltic pump) to maintain this particular flow if desired/required. Consequently, the inlet flow to the blood component collection device 18 typically includes both a flow of whole blood from the donor 14 and a flow of anticoagulant from the AC container 30.

The blood component collection device 18 separates the whole blood provided on line by the donor 14 into three primary constituents, namely platelets, a combination of red and white blood cells ("RBC/WBC"), and plasma. The platelets collected from the blood component device 18 are directed through a platelet collect line(s) 34 to one or more platelet collect bags 38 via a collect pump 36. The plasma and RBC/WBC are provided back to the donor 14 through a plasma line 42 and RBC/WBC line 46, respectively, both of which are interconnected with a second needle assembly (not shown) on the donor 14 via a donor return line 50. The plasma line 42 includes a plasma pump 40 (e.g., a peristaltic pump) to maintain the flow of plasma if desired/required. Although plasma may be provided back to the donor 14 in the above manner, it may be desirable to collect the separated plasma in some cases. In this regard, a plasma collect bag 54 may be provided and interconnected with the plasma line 42 (interconnection shown in phantom). In this case, appropriate valving 56 may be incorporated in the plasma line 42.

The blood component separation assembly 10" of Fig. 3 is similar to that of the dual needle configuration of Fig. 2 except that a single needle assembly (not shown) integrates the donor 14 within the blood component collection assembly 10". Consequently, similar components are similarly identified where appropriate. With regard to the single needle configuration of Fig. 3, whole blood of the donor 14 initially flows through a donor access line 62 and into an inlet line 66 which is fluidly connected with the blood component collection device 18 such that the platelets are separated and collected in the above-described manner. The plasma and RBC from the blood component collection device 18 flow through the plasma and RBC/WBC lines 42, 46, respectively, both of which are fluidly interconnected with a return flow controller 74. As above, however, the plasma may alternatively be directed to a plasma collect bag 54. In the event that plasma is not collected, the RBC/WBC and plasma are provided back to the donor 14 through the return flow controller 74 via a donor return line 70 which is interconnected with the donor access line 62. As can be appreciated, since only a single line is directly connected to the donor 14, namely the donor access line 62, blood is either being removed from or provided back to the donor 14 such that the procedure is effectively two-step versus continuous in relation to the donor 14.

5 The blood component collection device 18 used in the blood component collection assembly 10 is more particularly illustrated in Figs. 4A-B. This device 18 is the subject of U.S. Patent No. 4,387,848 to Kellog et al., entitled "CENTRIFUGE ASSEMBLY", issued June 14, 1983, and the disclosure of which is incorporated by reference in its entirety herein. This device 18 is also commercially available from the assignee of the present application as such is incorporated in COBE Spectra™.

10 Referring to Figs. 4A-B, the blood component collection device 18 utilizes a processing channel 80 to provide the desired disposable extracorporeal circuit. The channel 80 is positioned within a groove formed directly or indirectly in a centrifuge rotor (not shown) (e.g., a
15 separate filler may receive the channel 80 and be attached to the centrifuge rotor), and is illustrated in the shape which it assumes during processing (i.e., during flow of blood therethrough). All subsequent references herein to the structural and operational characteristics of the blood
20 component collection device 18 will be to the processing channel 80 in the illustrated condition.

The processing channel 80 generally includes a first stage 84 for collectively separating red blood cells ("RBC") and white blood cells ("WBC") from platelet-rich plasma, a second stage 92 for thereafter separating platelets from the platelet-rich plasma, a transition
25 portion 88 defining a separation between the first stage 84 and second stage 92, and a control chamber 124 for

17
maintaining a proper interface between the first stage 84 and second stage 92, namely the position of the interface between the RBC/WBC and platelet-rich plasma within the transition portion 88.

5 The first stage 84 extends from one end of the control chamber 124 along an arcuate path generally inwardly, toward the axis 132 about which the processing channel 80 rotates via the centrifuge rotor, until terminating at the transition portion 88. Specifically, the end of the first
10 stage 84 adjacent the control chamber 124 is positioned at a greater radial distance from the axis 132 than the end of the first stage 84 adjacent the transition portion 88. An inlet tube 96 is fluidly connected with the first stage 84 between its two ends to introduce whole blood into the
15 processing channel 80 and a RBC/WBC tube 100 is provided in the control chamber 124 for removing the separated RBC/WBC from the channel 80. Both the inlet tube 96 and RBC/WBC tube 100 extend externally of the rotatable device 18 for interconnection with the donor 14 and/or collection bags
20 38, 54.

As RBC/WBC sediment against the outer wall in the first stage 84 during rotation of the centrifuge rotor they are directed and counterflow toward the RBC/WBC tube 100 for removal from the channel 80 due to the increased
25 centrifugal forces at the RBC/WBC tube 100 in comparison with the transition portion 88. That is, since the first stage 84 extends along an arcuate path generally outwardly away from the axis 132 proceeding from the transition

portion 88 to the control chamber 124, the centrifugal force differential along the first stage 84 establishes the described counterflow of the separated RBC/WBC. Moreover, the transition portion 88 also assists in providing for this counterflow since it extends along an arcuate path generally inwardly toward the axis 132 proceeding from the first stage 84 to the second stage 92.

The platelet-rich plasma, which has a lower density than the RBC and WBC, flows beyond the transition portion 88 from the first stage 84 into the second stage 92 for further processing, while the RBC/WBC are directed back toward the RBC/WBC tube 100 in the above-described manner. The second stage 92 initiates at the radially inwardmost part of the transition portion 88 and extends along an arcuate path generally outwardly away from the axis 132 to a platelet collection chamber 104. Platelets are removed from the processing channel 80 at the platelet collection chamber 104 by a platelet tube 108 which interfaces with the outer wall of the processing channel 80 at the platelet collection chamber 104. Thereafter, the second stage 92 extends along an arcuate path generally inwardly toward the axis 132 until terminating at the plasma tube 112. Both the platelet tube 108 and plasma tube 112 extend externally of the rotatable device 18 for interconnection with the platelet collect bag(s) 38 and donor 14/plasma collect bag(s) 54, respectively.

Platelets which do not separate from the plasma in the initial portion of the second stage 92 between the transition portion 88 and platelet collection chamber 104 are separated in the portion of the second stage 92 between the platelet collection chamber 104 and the plasma tube 112. These platelets will flow back towards the platelet collection chamber 104 in the opposite direction of the flow of platelet-rich plasma/platelet-poor plasma through the second stage 92 due to the configuration of this portion of the second stage 92. That is, the platelet collection chamber 104 assumes the radially outwardmost position in the second stage 92 such that all platelets, regardless of where separation occurs in the second stage 92, flow towards the platelet collection chamber 104 for removal from the channel 80.

Platelet-poor plasma exits the second stage 92 and flows out through the plasma tube 112 which interfaces with the inner wall of the processing channel 80 and/or continues to flow through the remaining portion of the processing channel 80 to the control chamber 124. Plasma which flows to the control chamber 124 exits the channel through the control tube 114 which joins with the RBC/WBC tube 100 into a single outlet tube 120. The positionings and diameters of the RBC/WBC tube 100 and control tube 114 and the joinder of such into the common outlet tube 120 regulate the position of the RBC/WBC-platelet-rich plasma interface within the transition portion 88 using conservation of mass principles.

The blood component collection device 18 includes a prediction model 20 (appropriately interfaced with the operator input module 16 as shown in Fig. 1 as noted above and which may be used to configure the prediction model 20 and/or to allow operator input of various parameters to be used by the prediction model 20) for predicting a platelet yield before a collection procedure is initiated using a compilation of algorithms. The prediction model 20 may be used by the optimizer assembly 140 which is associated with principles of the present invention and thus will be briefly described herein. Notwithstanding the following discussion of the specifics of the prediction model 20, those skilled in the art will appreciate that the prediction model 20 is associated with the functional and operational characteristics of the blood component device 18 described herein. Therefore, the algorithms used in the prediction model 20 could and likely would vary in the case of other blood component collection devices which may be used by the present invention. Moreover, different algorithms could of course be used even for the prediction model 20. Furthermore, the algorithms are specific to platelet collection and therefore may and likely would change if used in relation to other blood component types such as red blood cells.

The prediction model 20 is typically configured by the site (e.g., the blood bank/center) for a particular blood component collection procedure (e.g., single or dual needle) used by the site and will be presented with regard

to the dual needle procedure of Fig. 2 and in relation to a platelet-collecting procedure. In this regard, an AC infusion rate (i.e., the rate at which anticoagulant is provided to the donor 14 per the blood volume of the donor 14) and the AC ratio (i.e., the collective flow of AC and blood through the inlet line 22 in relation to the flow of AC through the line 22) must be specified (through configuration or modified input as will be discussed below). Moreover, in the event that plasma is to be collected into the plasma collect bag 54 in the collection procedure, the maximum amount of plasma which should be collected considering the medical and physical characteristics of the donor 14 must also be provided.

There are two alternatives for establishing the plasma volume limit. The first alternative relating to the plasma volume limit is to provide a weight cutoff (e.g., 0-500 pounds), associated with the weight of the donor 14 which is input as will be discussed below. In this regard, a plasma volume upper limit (e.g., 10-1500 ml.) may be established for a weight of a donor 14 in excess of this cutoff, and a plasma volume lower limit (e.g., 10-1500 ml.) may be established for a weight of such donor 14 which is less than this cutoff. For instance, if the weight cutoff is 175 pounds, the plasma volume upper limit can be 600 ml. for a donor 14 weight greater than or equal to 175 pounds, and the plasma volume lower limit can be 500 ml. for a donor 14 weight less than 175 pounds.

The second alternative for a plasma volume limit is to configure the prediction model 20 such that the plasma volume limit is expressed as a percentage of the total blood volume of the donor 14 which is calculated pursuant to Eq. 10 below. For instance, the plasma volume limit may be established as 1-15% of the total blood volume of the donor 14, and is preferably established as about 12% of such volume.

Further information is required by the prediction model 20 prior to performing its yield prediction function. For instance, the total procedure time is typically input by the operator or preconfigured by the user (e.g., the blood bank/center). When configured the procedure time is typically 100 minutes. Moreover, the total procedure time is affected by whether a stepdown option is utilized for the blood component collection device 18 so as to enhance separation of the various blood components. When this stepdown option is selected, the angular velocity of the blood component collection device 18 is incrementally reduced during the platelet-collection procedure. For instance, the stepdown option could provide for angular velocities for the device 18 of 2400, 2200, and 2000 RPM, each of which would be for a specified duration.

Based upon the foregoing, the configuration of the prediction model 20 in relation to the blood component separation assembly 10' and associated protocol in effect standardizes site protocol for purposes of "normal" operations. However, for a particular donor 14 it may be

desirable to alter the "configuration" for one processing run. Consequently, the prediction model 20 utilizes a procedure in which certain parameters utilized in the following equations may be adjusted on a one-at-a-time basis. Such is referred to as modified input data and the associated parameters are procedure time (e.g., 10-999 minutes), inlet flow rate to the device 18 (e.g., 0-150 ml/min. for the Fig. 2 assembly and 0-50 ml/min. for the Fig. 2 assembly), AC ratio option as discussed above (3-50), the desired platelet collect volume (e.g., 10-9999 ml.), the desired platelet collect concentration (e.g., 100-8000 x 10⁶/ml.), and the desired source plasma volume to be collected (e.g., 0-9999 ml.). Moreover, other parameters such as AC infusion rate (0.8-1.1), stepdown option (yes or no), needle option (single or double), and high flow option (yes or no) may also be entered as modified input data by an operator.

Having configured the prediction model 20 in the above-described manner, the following additional information is provided and is utilized in the various calculations of Equations 1-22 presented below: (1) needle option, namely whether the procedure is dual needle (Fig. 2) or single needle (Fig. 3); (2) run identification number for purposes of associating the data/output generated by the various equations with a particular donor 14 and processing run; (3) the sex of the donor 14; (4) the height of the donor 14; (5) the weight of the donor 14; (6) the total blood volume as calculated in Eq. 10 below; (7) the

hematocrit of the donor 14, either based upon an initial estimation and thereafter updated based upon analysis of the donor's 14 blood sample (e.g., by a cell counter) or input directly from such an analysis; (8) the platelet precount, either based upon an initial estimation and thereafter updated based upon analysis of the donor's 14 blood sample (e.g., cell counter) or input directly from such an analysis; and (9) whether plasma collection is desired in conjunction with the platelet collection.

Based upon the above initial configuration and subsequent data input (except when entered as modified input data), the following output is generated by the prediction model 20: (1) platelet yield; (2) inlet flow rate; (3) AC ratio; (4) procedure time; (5) platelet collect volume; (6) platelet collect concentration; (7) source plasma volume; (8) AC in the platelet and plasma collect bags 38, 54; (9) platelet postcount; (10) AC infusion rate; and (11) output approval. This information is utilized at least in part in the following equations to generate, inter alia, the predicted platelet yield value of the collected platelets for the case of the dual needle procedure of Fig. 2 and also for the case of the single needle procedure of Fig. 3. The differences between those procedures with regard to the prediction model 20 are identified herein. As will be appreciated, some of the equations are utilized in the calculation of the predicted platelet yield, whereas other equations are used to generate additional information for output and

informational purposes. The variables or parameters and the units associated therewith of the equations are presented after the equations in the Variables Index.

5 Platelet Yield:

$$Y = 1 \times 10^6 C_{PR} V_B F_Y [1 - \exp[-E_c (f_{BP} - 0.12)]] \quad (\text{Eq. 1})$$

where:

$$f_{BP} = (Q_{IN} t_E + 50) (1 - 1/R) / V_B \quad (\text{Eq. 2})$$

and where:

$$Q_{IN} = RQ_{AC} = 0.001 I V_B PR \leq 150 \quad (\text{Eq. 3})$$

10

Alternatively, the platelet yield may be expressed as:

$$Y = 1 \times 10^6 C_{PR} V_B F_Y [1 - \exp[-E_c (0.001 I (R-1) P t_E + 50 (1 - 1/R) / V_B - 0.12)]] \geq 0 \quad (\text{Eq. 4})$$

Platelet Collection Efficiency:

$$E_c = C_1 - C_2 \exp [9.91 (1 - 1/R) H] Q_{IN} \geq 0 \quad (\text{Eq. 5})$$

where the constant C_1 is defined as follows:

$$\begin{aligned} C_1 &= 0.803 - \text{dual needle, without stepdown} \\ C_1 &= 0.840 - \text{dual needle, with stepdown} \end{aligned}$$

where the constant C_2 is defined as follows:

$$\begin{aligned} C_2 &= 4.08 \times 10^{-5} - \text{dual needle, without stepdown} \\ &\quad - \text{dual needle, with stepdown} \end{aligned}$$

and where:

$$Q_{INA} = Q_{IN} (t_E/t_P) \quad (\text{Eq. 6})$$

5

In Eq. 6, t_p may be provided as configuration data or modified data as provided above, or alternatively may be derived from the solution of Eq. 4 for t_e .

10 Effective Procedure Time:

$$\begin{aligned} t_E &= t_P, Q_{IN} \leq 45 \\ &= t_P - 500 (1/45 - 1/Q_{IN}), Q_{IN} > 45 \end{aligned} \quad (\text{Eq. 7})$$

Only high-flow protocol is used for $Q_{IN} > 45$.

AC Infusion Rate Constant:

$$I = 1000 Q_{IN} / (PRV_B) \quad (\text{Eq. 8})$$

15

Alternatively to the use of Eq. 8 for the derivation of the AC infusion rate constant I, such may be provided as configuration or modified input data pursuant to the above.

AC Ratio:

20

Initially, the AC ratio may be provided as configuration or modified input data pursuant to the above. In configuration, it is defined as follows:

$$\begin{aligned} R &= 1 + 2.51/H && \text{low} \\ &= 1.33(1 + 2.51/H) && \text{medium} \\ &= 1.67(1 + 2.51/H) && \text{high} \end{aligned} \quad (\text{Eq. 9})$$

25

Total Blood Volume:

$$V_B = 604 + 0.006012 L^3 + 14.6 W \text{ ml (male)} \quad (\text{Eq. 10})$$

$$= 183 + 0.005835 L^3 + 15.0 W \text{ ml (female)}$$

Plasma Collect Factor:

AC infusion rate control maintains the AC flow to the donor as:

$$Q_{ACD} = 0.001 I V_B \quad (\text{Eq. 11})$$

where the inlet flow associated with this is:

$$Q_{INO} = RQ_{ACD} = 0.001 IRV_B \quad (\text{Eq. 12})$$

Q_{IN} is proportional to the total AC flow, as given by Eq. 3, which includes the AC that flows to the platelet collect bag 38 and the plasma collect bag 54. P (Eq. 13) is the factor by which Q_{IN} is increased by collecting AC, relative to not collecting AC. That is,

$$P = Q_{IN}/Q_{INO} = (\text{average } Q_{AC})/Q_{ACD} \quad (\text{Eq. 13})$$

where:

$$P = 1 + (f_{ACP}/Q_{ACD}) [V_C/(t_P - 150/Q_{IN}) + V_{SP}/(t_P - 500/Q_{IN})] \quad (\text{Eq. 14})$$

and where:

$$f_{ACP} = [(R-1)(1-H)]^{-1} \quad (\text{Eq. 15})$$

Platelet Collect Volume:

$$V_C = 1 \times 10^{-4} Y / [C_B (1 + f_{ACP})] \quad (\text{Eq. 16})$$

Source Plasma Volume:

The four choices provided are as follows:

$$\left. \begin{aligned} V_{SP} &= 0 \\ &= V_{CON} - V_C \\ &= f_{SP} V_B - V_C \\ &= \text{specified as modified input} \end{aligned} \right\} \geq 0 \quad (\text{Eq. 17})$$

5

where:

$$\begin{aligned} V_{CON} &= V_{CONL}, W < W_C \\ &= V_{CONH}, W \geq W_C \end{aligned} \quad (\text{Eq. 18})$$

and where:

$$0.01 \leq f_{SP} \leq 0.15 \quad (\text{Eq. 19})$$

10

Donor Postcount:

$$C_{PO} = C_{PR} \exp[-E_C (0.001 I (R-1) P t_E + 50 (1-1/R) / V_B - 0.12)] \leq C_{PR} \quad (\text{Eq. 20})$$

A warning is given if $C_{PO} < 100$.

Collect Volumes:

$$V_{CB} = V_C (1 + f_{ACP}) \quad (\text{Eq. 21})$$

$$V_{SPB} = V_{SP} (1 + f_{ACP}) \quad (\text{Eq. 22})$$

15

The primary equation to be solved for purposes of the yield prediction by the prediction model 20 is Eq. 4. Consequently, Eqs. 1-3 and 5-22 are ancillary to Eq. 4 although they may be used to calculate other output data and/or information required by Eq. 4. With regard to the manner in which Eqs. 1-22 are solved, all the iteration loops are based on the technique of successive approximation, in which each iteration is a repeat of the previous one, but using updated parameter values calculated in the previous iteration. This process continues until all the convergence criteria are met. The convergence criteria are that, on successive iterations, the variable difference is ≤ 1 for V_c , ≤ 0.2 for t_e , and ≤ 10 for C_8 .

As noted above, the foregoing was based upon a dual needle configuration as illustrated in Fig. 2. In the event that a single needle configuration such as that illustrated in Fig. 3 is utilized, the following Eq. 7' is used in place of Eq. 7 and the constants C_1 and C_2 for Eq. 5 are as follows:

$$C_1 = 0.803$$

$$C_2 = 8.54 \times 10^{-5}$$

$$t_E = t_p, Q_{IN} \leq 20$$

$$= t_p - 215(1/20 - 1/Q_{IN}), Q_{IN} > 20 \quad (\text{Eq. 7'})$$

Variables Index

Symbols for Equations:

C_1, C_2 = constants in platelet collection efficiency equations

	C_B	= platelet concentration in collect bag, expressed as 10^3 platelets/microliter
5	C_{PO}	= donor postcount, expressed as 10^3 platelets/microliter
	C_{PR}	= donor precount, expressed as 10^3 platelets/microliter
10	E_C	= platelet collection efficiency
	f_{ACP}	= AC expressed as a fraction of pure plasma volume
15	f_{BP}	= fraction of V_B processed in platelet collection procedure
	f_{SP}	= V_{CON} expressed as a fraction of V_B
20	F_Y	= user-specific (e.g., blood bank/center) yield calibration factor
	H	= hematocrit of donor or patient
25	I	= AC infusion rate constant
	L	= donor or patient height, inches
30	P	= plasma collect factor
	Q_{AC}	= AC flow, ml/min
35	Q_{ACD}	= AC flow infused into donor for platelet collection procedures, ml/min
	Q_{IN}	= inlet flow, ml/min
40	Q_{INA}	= average inlet flow for platelet procedures, ml/min
	Q_{INO}	= RQ_{ACD} = inlet flow associated with Q_{ACD} , ml/min
45	R	= AC ratio
	t_E	= equivalent procedure time, min
	t_P	= procedure time, min
50	V_B	= total blood volume of donor or patient, ml
	V_C	= volume of pure plasma in platelet collect bag, ml
55	V_{CB}	= total volume in platelet collect bag, ml

V_{CON} = volume constraint for total pure plasma collected, ml
 V_{CONH} = higher value of V_{CON} , ml
 V_{CONL} = lower value of V_{CON} , ml
 V_{SP} = volume of pure plasma in source plasma bag, ml
 V_{SPB} = total volume in source plasma bag, ml
 W = donor or patient weight, lbs
 W_c = weight constraint associated with V_{CON} , lb
 Y = platelet yield, number of platelets.

As noted above, the optimizer assembly 140 associated with principles of the present invention interfaces with or at least provides information to one or more blood component collection assemblies 10 to provide a blood component collection system 2. That is, although there are definite advantages to having an interface between the optimizer assembly 140, particularly the optimizer module 144, and the blood component collection device 18, the optimization procedure may be performed at any location and input into the blood component collection device 18 in any manner. Since the general principles of the blood component collection assembly 10 were described with relation to the collection assemblies 10, 10" which included the blood component collection device 18 and its various features, the optimizer assembly 140 will be described in relation to such assemblies 10', 10". However, it will be appreciated that the fundamental

optimization principles of the present invention are not limited to these collection procedures and/or apparatus.

As noted (Fig. 1), the optimization assembly 140 generally includes a central input station 148, as well as an optimizer module 144 for each blood component collection device 18. Initially, it should be noted that the optimizer module 144 may be separate from the internal control of the blood component collection device 18 which is accessible by the operator interface module 16. However, typically the optimizer module 144 will be integrated with this internal control along with the above-described prediction model 20.

Referring to Fig. 5, the optimizer assembly 140 will be described with regard to a standard procedure. The central input station 148 will typically be used by blood banks/centers as the primary means for donor data input and donor data management. Information relating to a donor such as sex, height, weight, and demographics will be input at the central input station 148. Moreover, information relating to the donor's hematocrit and a blood component precount, both of which may be obtained from a donor blood sample and determined by known techniques such as cell counters, may also be entered at the central station 148. In addition to donor-related data, the particular type of collection procedure to be used for the donor (e.g., single needle or double needle) may be input/confirmed at the central input station 148. Based upon this information and certain site-standardized conditions (e.g., total procedure

time, collection efficiency, AC infusion rate), an initial procedure order is thereafter generated which specifies the various process control parameters associated with the selected collection procedure.

5 The initial procedure order may be transferred/down-
loaded onto the internal control of a blood component
collection device 18 by a computer disk 142 (Fig. 1) or
electronically if a network system is implemented (not
shown), through use of the operator interface module 16 if
10 required/desired. When this operator interface module 16
exists, it may of course be used for the initial donor data
input and/or to generate the initial procedure order and
thereby alleviate the need for a central input station 148.
However, it may be more efficient to use the central input
15 station. Although this initial procedure order may be used
in the collection process, the initial procedure order may
be optimized in accordance with principles of the present
invention to obtain one or more optimal values for the
process control parameters. As noted, this optimization
20 process may be utilized before the collection procedure is
actually initiated, but may also be initiated during a
given collection procedure and such is referred to as
downstream optimization.

25 With regard to the various optimization options,
process control parameters may be derived for a product-
based optimization. More particularly, the optimizer
assembly 140 and specifically the optimizer module 144
derives process control parameters for achieving a

predetermined yield of blood components through a maximization of at least one process parameter as will be discussed below in relation to the optimization models 152 (Fig. 6), 172 (Fig. 7). As noted above, in the United States a single platelet product (SPP) is 3×10^{11} platelets and a double platelet product (DPP) is 6×10^{11} platelets. Consequently, the optimizer module 144 may be configured to provide a number of product-based optimizations such as SPP and DPP. Although the exact values for a current U.S. SPP and DPP could be configured into the optimizer module 144, in order to increase the probability that the actual yield will equal or exceed the yield requirements for a current U.S. SPP or a DPP, the site may configure a SPP to be 3.5×10^{11} platelets and a DPP to be 7.0×10^{11} platelets (e.g., to effectively provide a given confidence level that the specified yield will actually be met).

The optimizer module 144 may also be configured to provide a time-based optimization. That is, for a given amount of time which a donor is available, the optimizer module 144 will derive those process parameters which allow for the collection of a "maximum" amount of platelets in this time period in relation to a maximization of at least one of the process control parameters.

Once the optimization is complete, the values for the various process control parameters generated thereby, as well any ancillary/previously specified values, are downloaded to the internal control of the blood collection device 18 such that the collection procedure may be

initiated or reinitiated (downstream optimization) as the case may be in accordance with these values. Once the procedure is completed, certain data is transferrable (via the disk 142 or electronically as noted) back to the central input station 148 for further use with regard to the particular donor. In addition, this information as well as the initial input may be used to generate various types of reports which may further assist in the management of the blood bank/center (e.g., individual run, donor/patient, summary reports). That is, this information may be used in the derivation of subsequent procedure orders for the particular donor. For instance, in the event that a certain AC infusion rate was used in the collection procedure which had certain effects on the donor, this may be recorded in the central input station 148 such that a lower AC infusion rate would be suggested/required for subsequent donations by the donor.

One model which may be incorporated into the optimization module 144 is illustrated in Fig. 6 and will be described with regard to platelet collections in accordance with the dual needle configuration of Fig. 2, although the module 144 may be used with a variety of other collection procedures and including the single needle configuration of Fig. 3, as well as with various other blood components. Initially, it should be noted that all references in Fig. 6 to "derivations" are actually provided by the prediction model 20 discussed above such that there is either an appropriate interface between the prediction

34

model 20 and optimizer module 144 or the optimization module 144 actually includes the prediction model 20. Moreover, as noted the prediction model 20 is specific to the blood component collection device 18 and to platelet collections. Therefore, if other devices are used the associated prediction model would also likely change as noted. Moreover, the associated prediction model may also vary in the case where different blood components such as red blood cells are to be collected.

10 The optimizer model 152 of Fig. 6 may be used for both product-based and time-based optimizations. Initially, the optimizer model 152 will be described with regard to a product-based optimization. That is, the fundamental premise of the optimization is to achieve a predetermined platelet (or other blood component type) yield (or within a yield range), preferably in the minimum amount of time.

15 The optimizer model 152 of Fig. 6 is comprised of four iterative loops. Generally, the first loop 156 is a derivation of an inlet flow (Q_{IN}) associated with a specified AC infusion rate (I_{SPEC}) which is typically set at a maximum value for purposes of the present invention and which is entered at the input station 154. This derivation is thereafter performed by the processing station 158 and includes the solution of Eqs. 4, 8, 14, and 16 and/or equations ancillary thereto by the prediction model 20 as discussed above.

There are of course various convergence criterion/ criteria which may be incorporated into the first loop 156. For instance, convergence may be based upon the current inlet flow (Q_{IN-C}) in the first loop 156 through use of a binary search technique. In this case, in solving the noted equations at the processing station 158 certain parameters remain fixed in the iterative derivation of the inlet flow (Q_{IN}) which achieves the specified AC infusion rate (I_{SPEC}) and these parameters are also specified at input station 154. These include the total blood volume (V_b) which can be calculated using Eq. 10 since the donor's height, weight, and sex are entered at the central input station 148, and the AC ratio (R), which can be calculated using Eq. 9 since the donor's hematocrit (H) has been determined, or may be specified at some value. Moreover, the total procedure time (t_p) remains fixed in each iterative derivation of the inlet flow (Q_{IN}) associated with the specified AC infusion rate (I_{SPEC}) in the first loop 156. However, since the total procedure time (t_p) is not known in the case of a product-based optimization and thus cannot be specified at the input station 154, a current total procedure time (t_{p-C}) initially will be assumed (e.g., this assumption is configured in the optimizer model 152 and since a range of total procedure times is provided in the prediction model 20 as noted above, the mean total procedure time (t_p) is typically configured into this portion of the optimizer model 152 as the initial current total procedure time (t_{p-C})). The "current" designation is

used for the total procedure time in this case since the optimizer model 152 provides for an adjustment of the total procedure time after each iterative determination of the inlet flow (Q_{IN}) which provides the specified AC infusion rate (I_{SPEC}) in the second loop 160 in order to achieve the desired yield (Y) if required in the case of a product-based optimization as will be discussed in more detail below.

Generally, the inlet flow-based binary search technique convergence may be provided by assuming a current value for the inlet flow (Q_{IN-C}), calculating a current plasma collect factor (P_C) using the current total procedure time (t_{P-C}), calculating a current AC infusion rate (I_C) using the current inlet flow (Q_{IN-C}) and current plasma collect factor (P_C), and adjusting the current inlet flow (Q_{IN-C}) (at the parameter update in the first loop 156) in accordance with the selected binary search technique until there is a predetermined convergence between the two most recent values for the current inlet flow (Q_{IN-C}) (i.e., wherein the difference between the two most recent values of Q_{IN-C} is less than some predetermined amount which means that the convergence criterion is met). In the case of a binary search technique, there will always be convergence (i.e., the convergence criterion will always be met) such that the optimizer model 152 will always exit the first loop 156 and enter the second loop 160.

As an alternative to the noted inlet flow-based convergence criterion/criteria and the noted binary search technique, another possibility is to base convergence on the specified AC infusion rate (I_{SPEC}) and use an iterative derivation to determine the desired inlet flow (Q_{IN}). In this case, the first loop 156 is used to once again iteratively derive the inlet flow (Q_{IN}) which provides the specified AC infusion rate (I_{SPEC}) at the processing station 158 from certain specified parameters. That is, the first loop 156 is still a maximization of the inlet flow (Q_{IN}) based upon the specified AC infusion rate (I_{SPEC}) which should be associated with the donor 14. This is again primarily through the solution of Eqs. 4, 8, 14, and 16 and/or equations ancillary thereto by the prediction model 20 discussed above.

For purposes of solving the above-identified equations in relation to the infusion rate-based convergence criterion, certain parameters remain fixed in the iterative derivation of the inlet flow (Q_{IN}) which achieves the specified AC infusion rate (I_{SPEC}) in the first loop 156 and these parameters are also specified at the input station 154. These include the specified AC infusion rate (I_{SPEC}) which is known and which is typically a maximum value for the donor 14, the total blood volume (V_s) which can be calculated using Eq. 10 since the donor's 14 height, weight, and sex are entered in the central input station 148, and the AC ratio (R) which can be calculated using Eq. 9 since the donor's 14 hematocrit (H) has been determined

and input in the central input station 148, or may be entered as modified input data. Moreover, the total procedure time (t_p) remains fixed in each iterative derivation of the inlet flow (Q_{IN}) associated with the specified AC infusion rate (I_{SPEC}). However, once again the total procedure time (t_p) is not known in the case of a product-based optimization and thus cannot be specified at the input station 154. Therefore, a current total procedure time ($t_{p,c}$) initially will be assumed (e.g., this assumption is configured in the optimizer model 152, and since a range of total procedure times is provided in the prediction model 20 as noted above, the mean total procedure time (t_p) is typically configured into the first loop 156 of the optimizer model 152). The "current" designation for the total procedure time is used for the above-identified reasons relating to the adjustment of the total procedure time in the second loop 160 if required to attain the desired yield (Y).

The solution of Eqs. 4, 8, 14, and 16 also requires that certain values be assumed for certain of the remaining parameters with still other parameters being derived from this assumption. In this case, an iterative procedure is used and updated/current values are used in the next iterative calculation(s). All parameters which change on each iteration of the first loop 156 are identified herein with a "c" subscript to designate that the most current value is to be used. Although the derivation of that inlet flow (Q_{IN}) which provides the specified AC infusion rate

(I_{SPEC}) may be accomplished in a variety of manners via Eqs. 4, 8, 14, and 16, one way is to assume a current value for the plasma collect factor (P_c), then calculate the current inlet flow (Q_{IN-C}) using the specified AC infusion rate (I_{SPEC}), then calculate the current yield (Y_c), then calculate the current plasma collection factor (P_c) using the current yield (Y_c), and repeat this procedure with the current values until there has been acceptable convergence on the current inlet flow (Q_{IN-C}) in relation to the specified AC infusion rate (I_{SPEC}) (e.g., when the particular convergence criterion/criteria is met/established). When there is acceptable infusion rate-based convergence, the optimizer model 152 exits the first loop 156 and enters the second loop 160. In order to offer protection for cases when there is no such convergence, a maximum number of iterations for the first loop 156 may be specified (not shown).

The second loop 160 of the optimizer model 152 is a total procedure time (t_p) iteration. That is, the second loop 160 is an iterative adjustment of the current total procedure time (t_{p-c}). Initially, in the second loop 160 and in the case of a product-based optimization the model 152 will never exit at the first comparator 162 since a total procedure time (t_p) is not specified at the input station 154. Consequently, the optimizer model 152 proceeds to the second comparator 166 where convergence criteria (i.e., more than one check) is made. One convergence criterion which is checked at the second comparator 166 is whether


the current yield (Y_c) is greater than or equal to the desired and specified yield (Y). In this case, the current yield (Y_c) may be calculated based upon the values specified at the input station 158, values derived at the processing station 158, and the current total procedure time (t_{p-c}) for comparison with the desired and specified yield (Y) (in some cases, this current yield calculation (Y_c) may have been performed in the first loop 156 and need not be repeated in the second loop 160). If the yield convergence criterion is met, the model 152 exits the second loop 160 and actually exits all the way through to the exit 151, as will be discussed below. In this case, the specified/derived values are "optimal" and the collection procedure could be performed on the device 18 using the noted values for the various control parameters.

In the event that the yield-based criterion is not met at second comparator 166, the second comparator 166 looks to a total procedure time-based convergence criterion which may be similar to that discussed above with regard to the inlet flow-based criterion (e.g., using a binary search technique with the convergence criterion then being a predetermined difference between the two most current values of the total procedure time (t_{p-c})). On the first time through the second loop 160 after the noted yield-based convergence criterion has failed and the total procedure time convergence criterion has failed, the current total procedure time (t_{p-c}) is adjusted and the model 152 returns to the first loop 156. That is, each time


that the current total procedure time (t_{p-c}) is adjusted in the second loop 160, the entirety of the first loop 152 is repeated (i.e., a new inlet flow (Q_{in}) associated with the specified AC infusion rate (I_{SPEC}) is derived using the current total procedure time (t_{p-c}) provided by the adjustment in the second loop 160). Other convergence criterion/criteria could be used in the second loop 160, such as specifying a maximum number of iterations to be performed by the second loop 160.

In the event that the yield-based convergence criterion is not met on the second loop 160 and the total procedure time-based convergence criterion is met at the second comparator 166 in the second loop 160, the optimizer model 152 exits the second loop 160 and enters the third loop 164. The third loop 164 is an iterative adjustment of the AC ratio (R). However, the model 152 initially enters the third comparator 169 where convergence criteria (i.e., more than one) are checked. One convergence criterion is again the above-noted yield-based convergence criterion.

15


20


25


30


If this yield-based convergence criterion is again not met, an AC ratio-based convergence criterion is checked at the third comparator 169. This may be similar to the inlet flow-based criterion discussed above (e.g., using a binary search technique with the convergence criterion being the two most current values of the AC ratio). On the first time through the third loop 164 after the yield-based criterion has failed and the AC ratio-based convergence criterion has failed, the AC ratio is adjusted and the

optimizer model 152 returns to the first loop 152. That is, each time that the AC ratio (R) is adjusted in the third loop 164, the entirety of the first and second loops 156, 160, respectively, is repeated. Other convergence criterion/criteria could be used in the third loop 164, such as specifying a maximum number of iterations of the third loop 164.

In the event that the yield-based convergence criterion is not met in the second or third loops 160, 164, respectively, and the second and third comparator 166, 169, respectively, and the AC ratio-based convergence criterion is met at the third comparator 169 in the third loop 164, the optimizer model 152 exits the third loop 164 and enters the fourth loop 168. The fourth loop 168 is an iterative adjustment of the specified AC infusion rate (I_{SPEC}). However, the optimizer model 152 initially enters the fourth comparator 170 where convergence criteria (i.e., more than one) are checked. One convergence criterion is the noted yield-based convergence criterion. If the noted yield-based convergence criterion is not met at the fourth comparator 170, an AC infusion rate-based criterion is checked at the fourth comparator 170. This may be similar to the inlet-flow based criterion discussed above (e.g., using a binary search technique with the convergence criterion being the two most current values of the AC infusion rate). On the first time through the fourth loop 168 after the yield-based criterion has failed and the AC infusion rate-based convergence criterion has failed, the

AC infusion rate is adjusted and the model 152 returns to the first loop 152. That is, each time that the specified AC infusion rate (I_{SPEC}) is adjusted, the entirety of the first, second and third loops 156, 160, 164, respectively, is repeated (with the AC ratio set back to its initial value as entered at the input station 154 on each iteration of the fourth loop 168). Other convergence criterion/criteria could be used in the fourth loop 168, such as specifying a maximum number of iterations of the fourth loop 168. In cases where the specified AC infusion rate (I_{SPEC}) is actually the maximum AC infusion rate, typically the fourth loop 168 will execute only a single time with a one-time increase in the AC infusion rate of, for instance, 20% (e.g., may be site-configured).

In the foregoing loops where a yield-based convergence criteria are identified, when the criteria are met the optimizer model 152 exits to exit 151 and the specified/derived (i.e., current) values for the various process control parameters may be provided to the device 18 for performing the collection procedure. However, there may be cases where no optimization occurs, such as when the optimizer model 152 exits to the exit 151 based upon the AC infusion rate based convergence criterion being met.

The optimizer model 152 may also be used for a time optimization. That is, the optimizer model will derive optimal process parameters for a predetermined total procedure time (t_p) through maximization of at least one of the process parameters in order to maximize the platelet

collection (or for other blood component types). In this case, the optimizer model 152 only executes the first loop 156 to derive the inlet flow (Q_{IN}) associated with a specified AC infusion rate (I_{SPEC}) (typically a maximum value) using the input total procedure time (t_p) in this iterative derivation instead of the assumed total procedure time (t_p) referenced above. Once there is acceptable convergence as defined above in the product-based optimization such that model 152 exits the first loop 156, the current yield (Y_c) may be calculated in the first loop 156 (but again may already have been calculated in the first loop 156 at the processing station 158 such that no further calculation is required) and the convergence criterion will be met at the first comparator 162 when entering the second loop 160 (i.e., in a time-based optimization when a total procedure time is specified at the input station 154, the model 152 will exit when entering the second loop 158). As a result, the inlet flow (Q_{IN}) and AC infusion rate (I) will be optimal and the collection procedure may be performed with such values.

Another optimization model is presented in Fig. 7 and may be used for both product-based and time-based optimizations. As in the case of the optimizer model 152, the optimizer model 172 may interface with the prediction model 20 or actually integrally incorporate the prediction model 20, and thus reference to Eqs. 1-22 will be further made herein. Generally, the optimizer model 172 is based upon the principle that optimization occurs when an optimal

inlet flow (Q_L) associated with an optimum system collection efficiency is used in the derivation of various process control parameters. Referring to Fig. 8, a representative inlet flow (Q_{IN})/yield (Y) curve is presented to show the optimal inlet flow (Q_L) associated with the maximum yield (Y_{MAX}). This optimal inlet flow (Q_L) is mathematically expressed by Eq. 23 presented below which results from differentiating Eq. 4 of the prediction model 20 with regard to the inlet flow (Q_{IN}). As can be appreciated, where different algorithms are used in the associated prediction model (whether based upon collection of blood components other than platelets, different collection apparatus, or alternative derivations of the various parameters with the same collection procedure and apparatus), the optimal inlet flow may be mathematically expressed in a different manner.

$$Q_L = \left(\frac{C_1}{2C_2} \right) e^{-9.91(1-1/R)H} - C_3 \quad (\text{Eq. 23})$$

$$C_3 = \frac{1}{2(t_p/K_7 - 1/K_9)} \quad \begin{array}{l} Q_o \geq 45 \text{ for Dual Needle ("DN")} \\ \geq 20 \text{ for Single Needle ("SN")} \end{array} \quad (\text{Eq. 24})$$

$$= 0, \quad \begin{array}{l} Q_o < 45 \text{ for DN} \\ < 20 \text{ for SN} \end{array} \quad (\text{Eq. 25})$$

$$\begin{array}{ll} K_7 = 500 \text{ (DN)} & K_9 = 45 \text{ (DN)} \\ = 215 \text{ (SN)} & = 20 \text{ (SN)} \end{array} \quad (\text{Eq. 26})$$

$$\begin{aligned} C_1 &= 0.803 \text{ (SN, DN without stepdown)} \\ &= 0.840 \text{ (DN with stepdown)} \end{aligned} \quad (\text{Eq. 27})$$

$$\begin{aligned} C_2 &= 4.08 \times 10^{-5} \text{ (DN)} \\ &= 8.54 \times 10^{-5} \text{ (SN)} \end{aligned} \quad (\text{Eq. 28})$$

Based upon the foregoing, the optimal inlet flow (Q_I) is really "optimal" in terms of the collection apparatus.

5 Referring again to Fig. 7, the optimizer model 172 will initially be described with regard to a product-based optimization wherein the desired yield (Y) is specified at input station 184. Generally, the inlet flow (Q_{IN}) associated with a specified AC infusion rate (I_{SPEC})

10 (typically the maximum AC infusion rate and also specified at input station 184) is iteratively derived from certain other specified parameters. This inlet flow calculation, particularly when the maximum AC infusion rate (I_{MAX}) and maximum AC ratio (R_{MAX}) are specified, the inlet flow (Q_{IN}) is

15 optimal based on the physiological considerations of the donor 14. This is primarily through the solution of Eqs. 4, 8, 14, and 16 and/or equations ancillary thereto by the prediction model 20 discussed above. For purposes of solving these equations certain parameters remain fixed in

20 the iterative derivation of the inlet flow (Q_{IN}) which achieves the specified AC infusion rate (I_{SPEC}) and these parameters are also specified at input station 184. These include the total blood volume (V_B) which can be calculated using Eq. 10 since the donor's height, weight, and sex are

entered in the central input station 148, and the AC ratio (R), which can be calculated using Eq. 9 since the donor's hematocrit (H) has been determined, or may be specified at some maximum value. Moreover, the total procedure time (t_p) remains fixed in each iterative derivation of the inlet flow (Q_{IW}) associated with the specified AC infusion rate (I_{SPEC}). However, since the total procedure time (tP) is not known in the case of a product-based optimization and thus cannot be specified at the input station 184, a current total procedure time ($t_{p,c}$) initially will be assumed (e.g., this assumption is configured in the optimizer model 172 and since a range of total procedure times is provided in the prediction model 20 as noted above, the mean total procedure time (t_p) is typically configured into this portion of the optimizer model 172 as the initial current total procedure time ($t_{p,c}$)). The "current" designation is used for the total procedure time in this case since the optimizer model 172 provides for an adjustment of the total procedure time after each iterative determination of the inlet flow (Q_{IW}) which provides the specified AC infusion rate (I_{SPEC}) in order to achieve the desired yield (Y) if required in the case of a product-based optimization as will be discussed in more detail below.

The solution of Eqs. 4, 8, 14, and 16 also requires that certain values initially be assumed for certain of the remaining parameters. In this case, an iterative procedure is used in the solution of the yield equation (Eq. 4) (and including equations ancillary thereto as noted above) and

updated values are used in the next iterative calculation(s) at the processing station 188. Although the derivation of that inlet flow (Q_{IN}) which provides the specified (typically maximum) AC infusion rate (I_{SPEC}) may be accomplished in a variety of manners via Eqs. 4, 8, 14, and 16, one way is to assume a current value for the plasma collect factor (P), then calculate the current inlet flow (Q_{IN-C}) using the specified AC infusion rate (I_{SPEC}), then calculate the current yield (Y_C), then calculate the current plasma collection factor (P_C) using the current yield (Y_C), and repeat the foregoing with the updated parameters, all within the processing station 188, until there has been acceptable convergence on the current inlet flow (Q_{IN-C}) in relation to the specified AC infusion rate (I_{SPEC}).

In addition to the calculation of the current inlet flow (Q_{IN-C}) associated with the specified AC infusion rate (I_{SPEC}), the above-discussed optimal inlet flow (Q_L) is calculated at processing station 192. Consequently, a comparison can be made between the current inlet flow (Q_{IN-C}) which was derived in the above-described manner and the optimal inlet flow (Q_L) at the first comparator 176. If the current inlet flow (Q_{IN-C}) is less than the optimal inlet flow (Q_L) at the first comparator 176, the specified values for the various parameters associated with the inlet flow Q_{IN} are "optimum", namely the AC ratio (R) and the AC infusion rate (I) specified at the input station 184. Thereafter, the current yield (Y_C) (which was calculated in the derivation of the current inlet flow (Q_{IN-C}) associated

with the specified AC infusion rate (I_{SPEC}) at the processing station 188) is compared with the input yield (Y) at second comparator 180. In the event that there has been acceptable convergence between these yield values, the current total procedure time (t_{p-c}) is also "optimal". However, in the event that there has not been acceptable convergence between these yield values, the current total procedure time (t_{p-c}) is adjusted at adjusting station 196 and the foregoing iterative derivation of the current inlet flow (Q_{IN-C}) associated with the specified AC infusion rate (I_{SPEC}) is repeated until such convergence is achieved (i.e., using the initially specified AC infusion rate (I_{SPEC}) and the now adjusted current total procedure time (t_{p-c} , a new current inlet flow (Q_{IN-C}) is iteratively derived in the above-described manner).

Referring back to the first comparator 176, if the current inlet flow (Q_{IN-C}) associated with the specified AC infusion rate (I_{SPEC}) derived at processing station 188 is greater than the optimal inlet flow (Q_o), a current AC infusion rate (I_c) associated with this particular inlet flow (Q_o) is iteratively derived at the processing station 188 generally in the above-described manner (i.e., the initially specified AC infusion rate (I_{SPEC}) is disregarded in this derivation and a current AC infusion rate (I_c) is iteratively derived to coincide with the inlet flow (Q_o)). In this case, the current inlet flow (Q_{IN-C}) will always be equal to the optimal inlet flow (Q_o) at the first comparator 176 and the optimizer model 172 thereafter proceeds to the

second comparator 180 for the yield comparison in accordance with the above-described procedure.

The optimizer model 176 may also be used for a time-based optimization. In this case, the total procedure time (t_p) is specified at the input station 184 as a specified total procedure time (t_{p-spec}) and thus is not assumed as in the product-based optimization. The optimizer model 172 thereafter proceeds in the same manner discussed above with regard to the product-based optimization except at the second comparator 180. Since no yield was input there is no yield comparison made at the second comparator 180. Instead a total procedure time comparison is made at the second comparator 180. Since the current total procedure time (t_{p-c}) was set equal to the specified total procedure time (t_{p-spec}) prior to the model 172 proceeding to the processing station 188 in this time-based optimization, the model 172 will exit each time at the second comparator for a time-based optimization.

In addition to the above-described product-based and time-based optimizations, the principles of the present invention may be extended to other applications relating to enhancing blood component system management. For instance, an optimization in accordance with principles of the present invention may be extended to encompass donor management issues. In one such case, another "optimization" associated with the blood component collection process would be to collect blood components as dictated by existing inventory (i.e., use optimization as

dictated by existing inventory (i.e., use optimization as an inventory control). That is, information relating to the inventory of the various types of blood components in the blood bank/center and/or the demand for one or more blood component types could be maintained such that specific collection procedures could be selected to accommodate for a low supply of a given blood component type and/or a high demand for such blood component type. More specifically, in the event that the supply of red blood cells was low and/or the demand for red blood cells was high, or anticipated to be so in the near future, prompts could be provided to operators that red blood cells should be selected for collection if possible from donors during a given time period. Relatedly, the optimization principles of the present invention would be applicable to maintaining data on blood component collections from a given donor such that a determination could be made as to what type or types of blood components from the particular donor provided the maximum yield in the collection procedure. That is, information could be collected and maintained from prior blood component donations such that a determination could be made for a specific donor as to which type or types of blood components the donor has had a propensity to produce maximum yields therefor.

Notwithstanding the foregoing description of the present invention in relation to an on-line blood component collection process, those skilled in the art will appreciate that the source of blood may be provided to the

blood component collection device from an appropriate blood container (not shown) interconnected with the blood component collection device 18 versus receiving such directly from the donor. Moreover, the blood of course may be provided from alternative sources such as animals. Furthermore, as illustrated in Fig. 3 the described platelet harvesting procedure may be performed utilizing a single needle configuration. In addition, the present invention is applicable to the collection of other types of blood components such as red blood cells, white blood cells, and/or plasma, and is further applicable to the simultaneous collection of more than one blood component type. In the case of red blood cell collection and optimization in accordance with principles of the present invention, the donor's blood type should be known and used in various algorithms. Moreover, the present invention is not limited to the source being whole blood. That is, the principles of the present invention may be applicable to removal of a component from any liquid.

The foregoing description of the present invention has been presented for purposes of illustration and description. Furthermore, the description is not intended to limit the invention to the form disclosed herein. Consequently, variations and modifications commensurate with the above teachings, and skill and knowledge of the relevant art, are within the scope of the present invention. The embodiments described hereinabove are further intended to explain best modes known of practicing

the invention and to enable others skilled in the art to utilize the invention, and such other embodiments, and with various modifications required by the particular applications or uses of the present invention. It is intended that the appended claims be construed to include alternative embodiments to the extent permitted by the prior art.

5

D
B
P

S

E

T

THE CLAIMS DEFINING THE INVENTION ARE AS FOLLOWS:

1. A method for collecting at least one predetermined type of blood component from a source of whole blood using a blood component collection system comprising a blood component collection device and collection procedure, said collection procedure having a plurality of parameters associated therewith, said method comprising the steps of:
- 10 providing biological data relating to a source of whole blood, said source being a human donor and said data comprising at least one of said donor's hematocrit, height, weight, and sex;
- 15 identifying a desired yield of at least one predetermined type of blood component;
- 20 associating a magnitude with each of a plurality of parameters associated with a collection procedure to be performed on said whole blood using a blood component collection system comprising a blood component collection device and said collection procedure, said associating step comprising performing a first deriving step comprising deriving a magnitude for at least one of said parameters from said providing and identifying steps;
- 25 inputting said magnitude of each said parameter into said blood component collection system after said associating step; and
- 30 performing said collection procedure on said blood component collection device using said inputting step to collect said desired yield of said at least one predetermined type of blood component from said source of whole blood.
2. A method, as claimed in Claim 1, wherein: said biological data comprises said donor's hematocrit, height, weight, and sex.
- 35 3. A method, as claimed in Claim 1, wherein: of said parameters is an inlet flow to said blood collection device and another of said parameters is a flow



of anticoagulant into said blood component collection system, wherein said inlet flow comprises a flow of whole blood from said source and said flow of anticoagulant, wherein said source of said blood has a volume, wherein an
5 AC ratio is a ratio of said inlet flow to said flow of anticoagulant, and wherein an AC infusion rate is a flow of said anticoagulant provided to said source per said volume of said source.

4. A method as claimed in any one or Claims 1-3
10 characterized in that said performing a first deriving step further comprises:

deriving said magnitude of said inlet flow associated with a predetermine magnitude of said AC infusion rate.

15 5. A method as claimed in Claim 4, characterised in that said deriving said magnitude of said inlet flow step comprises:

using said predetermine magnitude of said AC infusion rate and a current magnitude for a total procedure time, said total procedure time being another of said
20 parameters.

6. A method as claimed in Claim 5, wherein said deriving said magnitude of said inlet flow step further comprises:

25 assuming a current magnitude for said inlet flow and performing a first iteration procedure comprising calculating a current magnitude for said AC infusion rate from at least said current magnitude of said inlet flow, evaluating convergence criteria relating to said current
30 magnitude of said inlet flow, and adjusting said current magnitude of said inlet flow, repeating said first iteration procedure until at least one of first and second conditions is satisfied, said first condition being that said convergent criteria is established and said second
35 condition being that said first iteration procedure has been performed a predetermine number of times.

7. A method, as claimed in Claim 5, wherein:



said deriving said magnitude of said inlet flow step comprises deriving a current magnitude for said AC infusion rate, said performing a first deriving step further comprising iteratively calculating a current blood
5 component yield using at least said current magnitude of said inlet flow and said current magnitude of said AC infusion rate and by using said providing step and by iteratively adjusting said magnitude of said current total procedure time until achieving at least one of first and
10 second conditions, said first condition being within a predetermine variance of said desired yield of blood components and said second condition being performing said iteratively adjusting step a predetermine number of time.

8. A method as claimed in Claim 6, wherein:

15 said deriving said magnitude of said inlet flow step comprises deriving a current magnitude for said AC infusion rate, said performing a first deriving step further comprising performing a second iteration procedure after said at least one of said first and second conditions
20 is satisfied, said second iteration procedure step comprising calculating a current yield from said current magnitude of said inlet flow, said current magnitude of said AC infusion rate, and said current magnitude of said procedure time, comparing said current yield with said
25 desired yield, performing said inputting step after said comparing step when said current yield is within a predetermined amount of said desired yield, adjusting said current magnitude of said total procedure time when said current yield differs from desired yield by more than said
30 predetermined amount, repeating said deriving a magnitude of said inlet flow step after said adjusting said current magnitude of said total procedure time step, and repeating said second iteration procedure step after said repeating said deriving a magnitude of said inlet flow step until at
35 least one or third and fourth conditions is satisfied, said third condition being that predetermine convergence criteria relating to said current total procedure time is



established and said fourth condition being that said second iteration procedure step has been performed a predetermined number of times.

5 9. A method, as claimed in Claim 5, wherein said performing a first deriving step further comprises deriving a total procedure time, after said deriving said magnitude of said inlet flow step, which provides a current yield within a predetermine amount of said desired yield.

10 10. A method, as claimed in Claim 8, wherein:
said performing a first deriving step further comprises performing a third iteration procedure after said second iteration procedure step and when said at least one of said third and fourth conditions is satisfied, said third iteration procedure step comprising adjusting said
15 magnitude of said AC ratio, repeating said first and second iteration procedure steps, and repeating said third iteration procedure step until at least one of fifth and sixth conditions is satisfied, said fifth condition being that predetermined convergence criteria relating to said
20 magnitude of said AC ratio is established and said sixth condition being that said third iteration procedure step has been performed a predetermined number of times.

25 11. A method, as claimed in Claim 10, wherein:
said predetermined magnitude of said AC infusion rate is increased by a predetermine amount when at least one of said fifth and sixth conditions associated with said third iteration procedure step is satisfied, wherein said performing a first deriving step further comprises repeating a first, second, and third iteration procedure
30 steps using said increased AC infusion rate.

12. A method as claimed in any one of Claims 3-11 characterized in that:

35 said associating step comprises selecting a maximum magnitude for said AC infusion rate, and wherein said associating step further comprises generating a calculated magnitude of said inlet flow using at least said maximum magnitude of said AC infusion rate.



13. A method as claimed in Claim 12,
characterized in that:

said performing a first deriving step further
comprises:

5 calculating a theoretical magnitude of said inlet
flow which provides a maximum yield of said at least one
predetermined blood component and comparing said
theoretical and calculated magnitudes of said inlet flow
and wherein said inputting step comprises inputting the
10 lesser of said theoretical magnitude and said calculated
magnitude of said inlet flow.

14. A method, as claimed in Claim 13, wherein:
one of said parameters is total procedure time,
wherein a current magnitude for said total procedure time
15 is assumed, and wherein said performing a first deriving
step further comprises performing a first iteration
porcedure step comprising calculating a current blood
component yield using the lesser of said calculated and
theroretical magnitudes of said inlet flow of whole blood,
20 said current magnitude of said total porcedure time, and
said maximum AC infusion rate, comparing said current blood
component yield with said desired blood component yield,
and repeating said first iteration procedure step using an
adjusted current total procedure time until at least one or
25 first and second conditions is staisfied, said first
condition being that said current magnitude of said blood
component yield is within a predetermined amount of said
desired blood component yield and said second condition
being that said peforming a first iteration procedure step
30 has been performed a predetermined number of times.

15. A method as claimed in Claim 13, wherein:
one of said parameters is a total procedure time
and said performing a first deriving step further comprises
assuming a current magnitude for said total procedure time
35 and performing a first iteration procedure, said performing
a first iteration procedure step comprising calculating a
current yield from the lesser of said actual and



theoretical magnitudes of said inlet flows, a maximum magnitude for said AC ratio, said maximum magnitude of said AC infusion rate, and said current magnitude of said procedure time, comparing said current yield with said
5 desired yield, incrementally adjusting said current magnitude of said total procedure time when said current yield differs from desired yield by more than a predetermined amount, and repeating said first iteration procedure step until at least one or a first and second
10 condition is satisfied, said first condition being that said current yield is within said first predetermined amount of said desired yield and said second condition being that said first iteration procedure step has been performed a predetermined number of times.

15 16. A method, as claimed in any one of Claims 3-15 characterized in that:

said at least one of said parameters is a total procedure time, said performing a first deriving step comprising maximizing said inlet flow and minimizing said
20 total procedure time.

17. A method as claimed in any one of Claims 1-16, characterized in that:

providing a magnitude for each of said parameters before said identifying step;

25 performing said collection procedure on said blood component collection device before said identifying step, using said providing a magnitude step, and for a first time period, wherein said associating step is performed after expiration of said first time period.

30 18. A method as claimed in any one of Claims 1-17 characterized in that:

one of said parameters is a total procedure time, and wherein said performing a first deriving step comprises minimizing said magnitude of said total procedure time
35 based upon said magnitude of at least one of said parameters other than said total procedure time.

19. A method, as claimed in Claim 18,



characterized in that:

one of said parameters is an inlet flow to said blood collection device and another of said parameters is a flow of anticoagulant into said blood component collection system, wherein said inlet flow comprises a flow of whole blood from said source and said flow of anticoagulant, wherein said blood within from said source has a volume, wherein at least part of said flow of anticoagulant is provided to said source, wherein an AC ratio is a ratio of said inlet flow to said flow of anticoagulant, wherein an AC infusion rate is said at least part of said flow of anticoagulant per said volume, and wherein said at least one of said parameters associated with said minimizing step comprises said magnitude of said AC infusion rate and said magnitude of said inlet flow.

20. A method, as claimed in any one of claims 1-19, characterized in that:

said associating step comprises optimizing said magnitude of at least one of said parameters.

21. A method for collecting a blood component from a source of whole blood using a blood component collection system comprising a blood component collection device and collection procedure, wherein an inlet flow to said blood component collection system comprises a flow of whole blood from said source and a flow of anticoagulant, said method comprising the steps of:

identifying a total procedure time for a collection procedure to be performed on a source of whole blood to obtain a plurality of at least one type of blood component therefrom using a blood component collection system comprising a blood component collection device and said collection procedure;

deriving a first inlet flow to said collection system which provides a maximum yield of said blood components;

deriving a second inlet flow to said collection system using at least said identifying a total procedure



time step;

identifying a smallest magnitude of said first and second inlet flow as an actual inlet flow to said blood component collection system; and

5 performing said collection procedure with said blood component collection device, using said actual inlet flow, and for said total procedure time to collect said blood components from said source of whole blood.

22. A method, as claimed in Claim 21,
10 characterized in that:

said blood within said source has a volume, wherein at least part of said flow of anticoagulant is provided to said volume, wherein an AC ratio is a ratio of said inlet flow to said flow of anticoagulant, wherein an
15 AC infusion rate is said at least part of said flow of anticoagulant per said volume, and wherein said deriving a second inlet flow step further uses a maximum AC ratio and a maximum AC infusion rate.

23. A method for collecting a blood component
20 from a donor using a blood component collection system comprising a blood component collection procedure and a collection procedure, said collection device comprising a plurality of parameters, said method comprising the steps of:

25 providing biological data relating to a donor;
associating a magnitude with a plurality of control parameters associated with a collection procedure to be performed on blood from said donor to obtain a plurality of at least one type of blood component therefrom
30 using a blood component collection system, said blood component collection system comprising a blood component collection device and said collection procedure, said associating step being based upon at least said providing step;

35 optimizing said magnitude of at least one or said control parameters in relation to both donor constraints and system constraints, said optimizing step allowing for



achieving at least one of first and second conditions, said first condition being collecting a predetermined quantity of said blood components in a minimum amount of time and said second condition being collecting a maximum quantity of said blood components in a predetermined amount of time; 5
inputting said magnitudes of said parameters into said blood component collection device after said optimizing step; and

performing said collection procedure on said 10
blood component collection device using said parameters to collect said blood components from said donor to achieve at least one of said first and second conditions.

24. A blood component collection control and information communication system used in conjunction with a 15
blood component collection device in a procedure performed on a donor to separate, remove and collect components from blood received from the donor, comprising:

an information communication medium;
a first station interactive with the 20
communication medium to transmit and receive information on the medium describing biological data of the donor, describing process parameters for controlling the collection device during the procedure performed on the donor, describing physical and medical characteristics of 25
the donor observed during performance of a prior procedure on the donor, and describing the yield of at least one component obtained from the donor during performance of the procedure; the first station including an information input device by which to supply donor data, process parameters, 30
prior procedure characteristics and component yield information to communication medium; the first station further including a computer responsive to the donor data, prior procedure characteristics and component yield information received from the communication medium to 35
determine at least one process parameter to be used for controlling the blood component collection device during performance of a subsequent procedure on the donor; and the



first station also including a display by which to display the donor data, process parameters, prior procedure characteristics and component yield information;

a second station interactive with the
5 communication medium to transmit and receive information on the medium describing biological data of the donor, describing process parameters for controlling the collection device during the procedure performed on the donor, describing physical and medical characteristics of
10 the donor observed during performance of a prior procedure on the donor, and describing the yield of at least one component obtained from the donor during performance of a procedure; the second station including an information input device by which to supply donor data, process
15 parameters, prior procedure characteristics and component yield information to communication medium; the second station further including a computer responsive to the donor data, prior procedure characteristics and component yield information received from the communication medium to
20 determine at least one process parameter to be used for controlling the blood component collection device during performance of a subsequent procedure on the donor; and the second station also including a display by which to display the donor data, process parameters, prior procedure
25 characteristics and component yield information; and
an interface of at least one of the first or second stations which connects to the blood component collection device to the one station, the interface
adaptable for controlling the blood collection device to
30 perform the procedure in response to the process parameter information transmitted to the one station by the communication medium; the interface further supplying information to the medium at the one station describing the yield of at least one component obtained from the donor
35 during performance of the procedure performed.

25. A method of controlling a blood component collection device in a procedure performed on a donor to

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50



separate, remove and collect components from blood received from the donor and for communicating information describing the procedure, comprising the steps of:

5 establishing first and second stations, each of which includes a computer, an information input device and a display;

connecting one of the first and second stations to the blood component collection device;

10 communicating information between the first and second stations which describes biological data of the donor, process parameters for controlling the collection device during the procedure performed on the donor, physical and medical characteristics of the donor observed during performance of a prior procedure on the donor, and
15 the yield of at least one component obtained from the donor during performance of the procedure;

using the information input device at either the first or the second station to create at least some of one of the donor data information, the process parameter
20 information, the prior procedure characteristics information and the component yield information;

deriving at least some of the process parameter information by processing the donor data, prior procedure characteristics and component yield information with the
25 computer at one of the first or second stations; and

controlling the operation of the blood component collection device in response to the process parameter information which was communicated, created by using the information input device and derived from the computer.

30 Dated this 23rd day of July 1997

COBE LABORATORIES, INC.

By their Patent Attorneys

GRIFFITH HACK

Fellows Institute of Patent

35 Attorneys of Australia



ABSTRACT

A blood component collection system with optimization capabilities. In one embodiment, process parameters are derived from an input/configured predetermined blood component yield and which is based upon the maximization of at least one process parameter. Thereafter, the blood component collection procedure is performed with these derived process control parameters. In another embodiment, process parameters are derived from an input total procedure time from a maximized value for at least one of the other process control parameters so as to maximize blood component yield in this fixed time. Thereafter, the blood component collection procedure is performed with these derived parameters.



11 10 9 75723

1/9

75723/94

FIG. 1


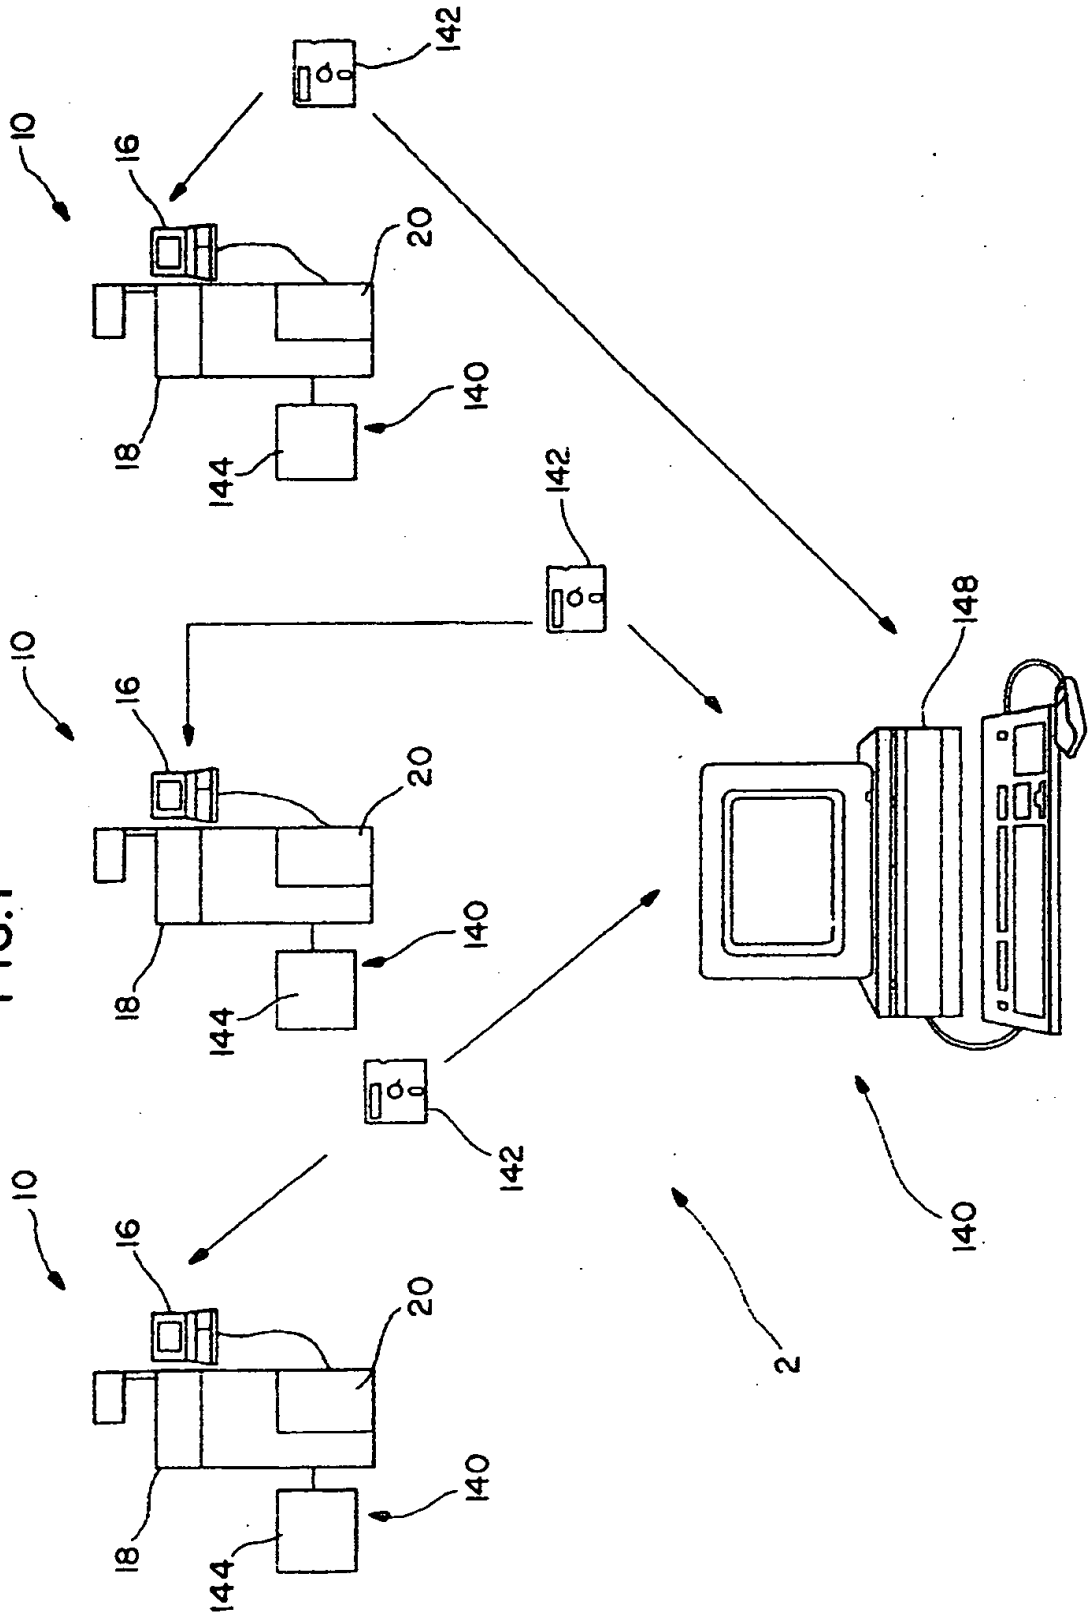


FIG. 2

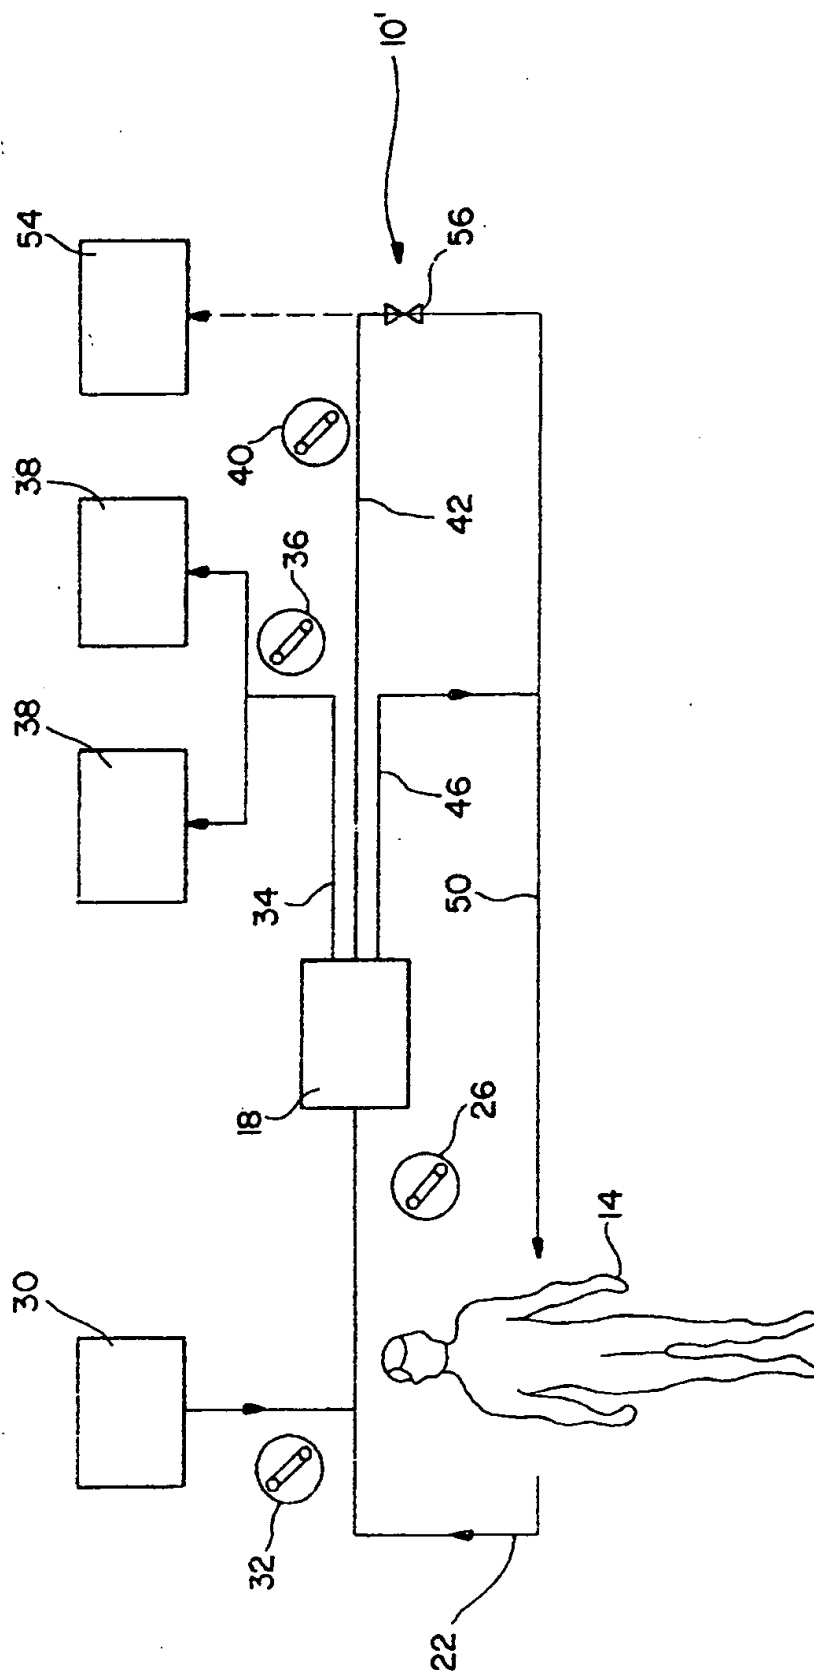

11 10 9 8 7 6 5 4 3 2 1

FIG. 3



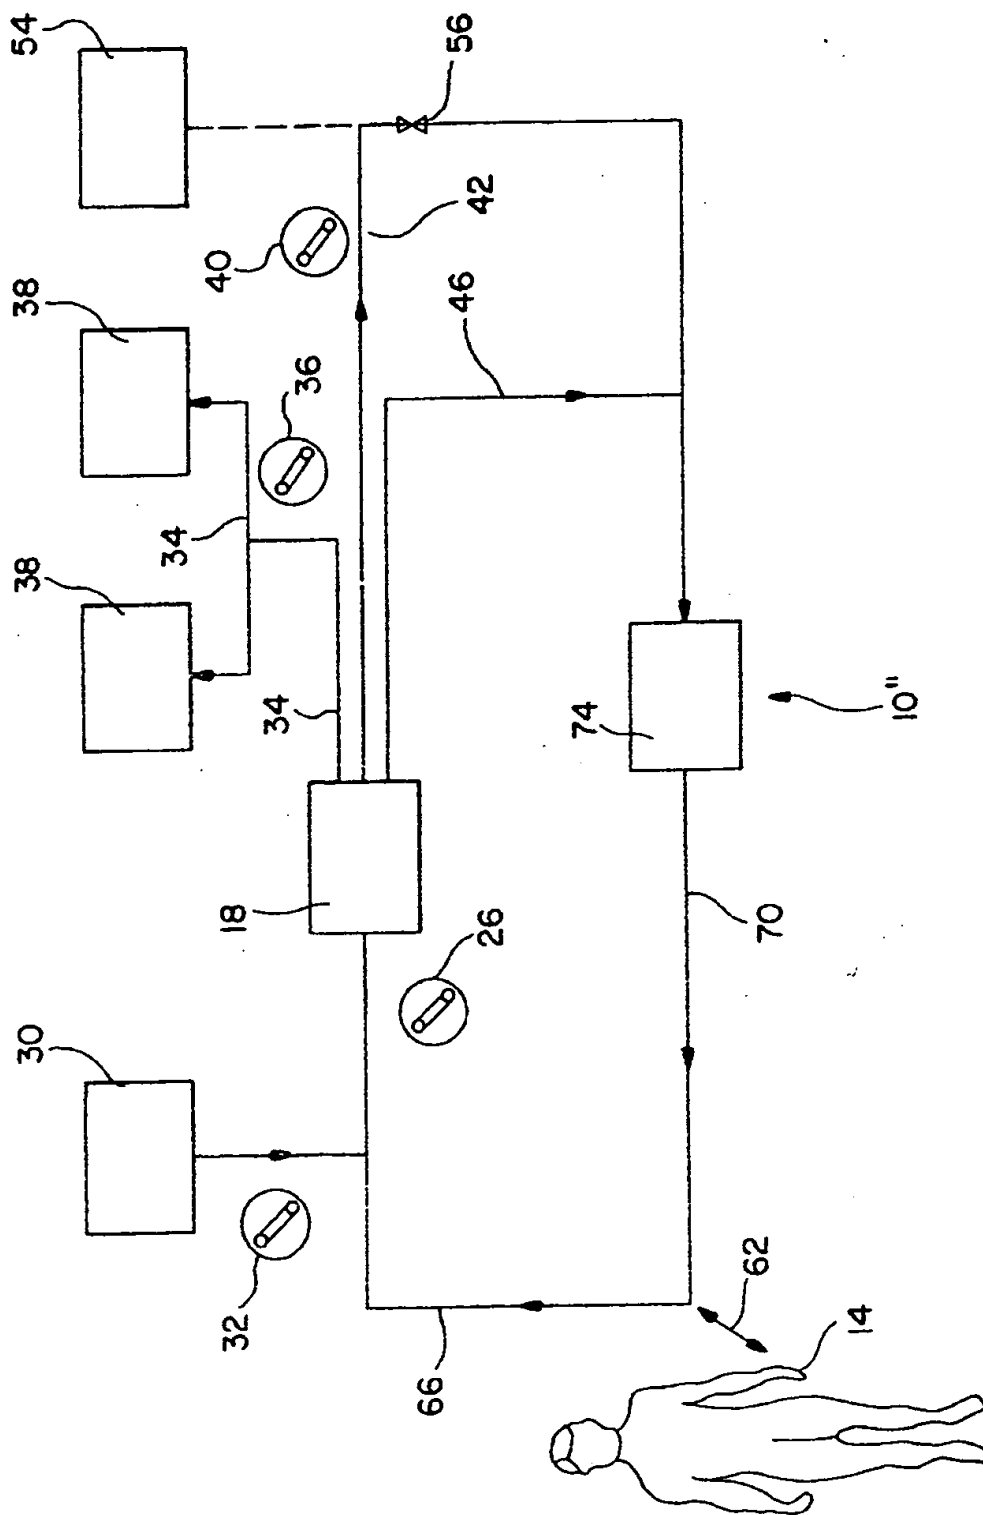


FIG. 4A

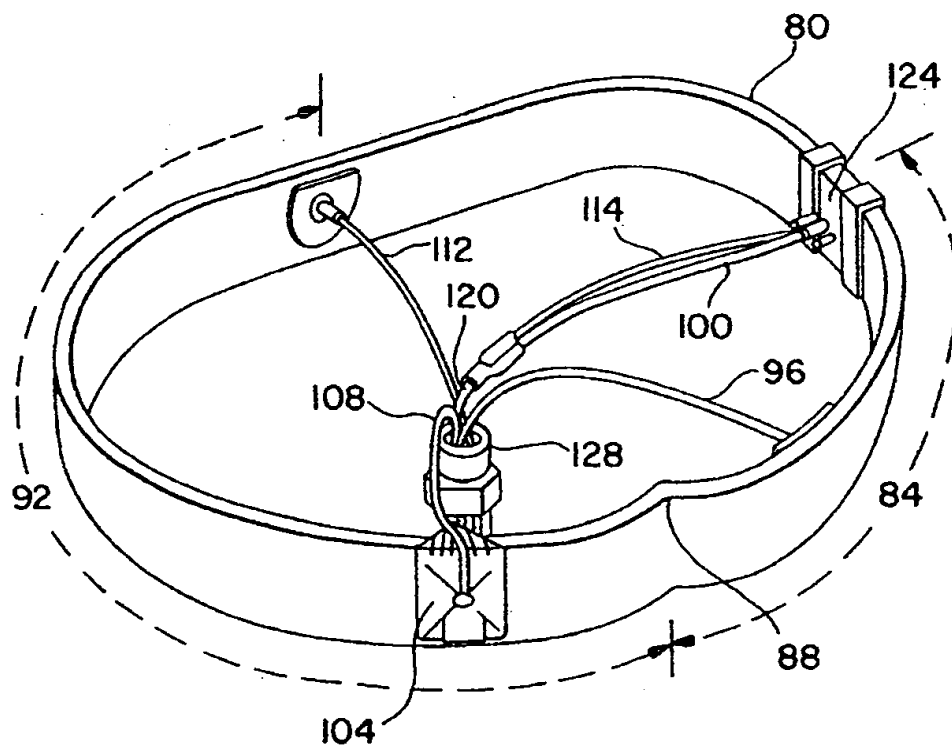


200
200
200
200
200

FIG. 4B

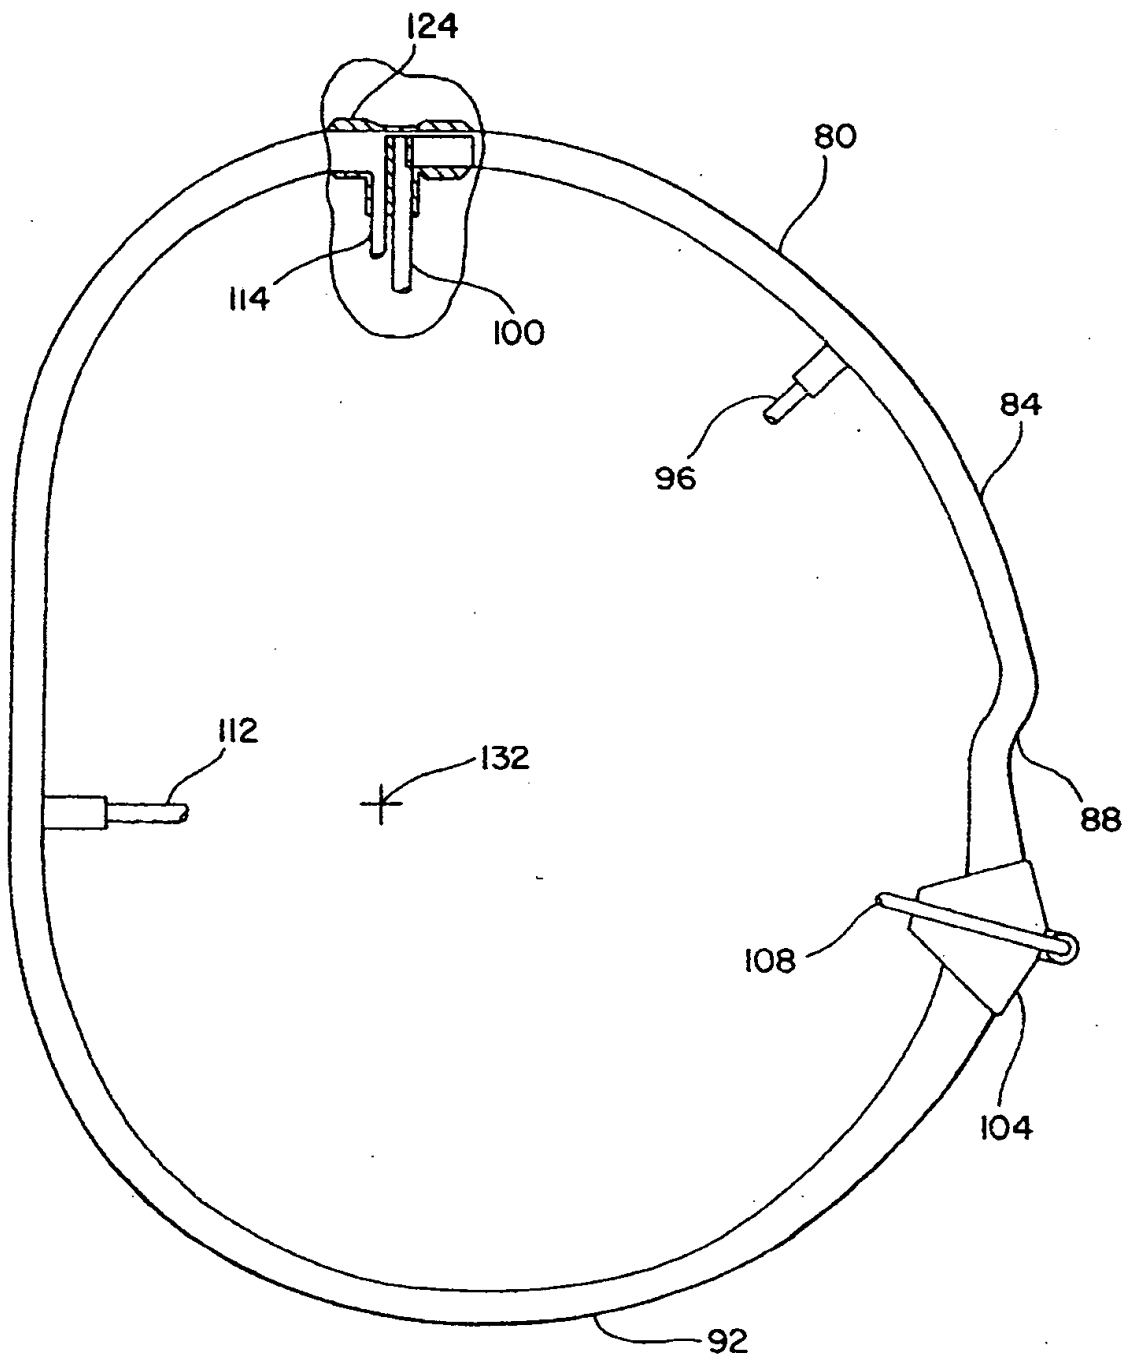

2025

FIG.5

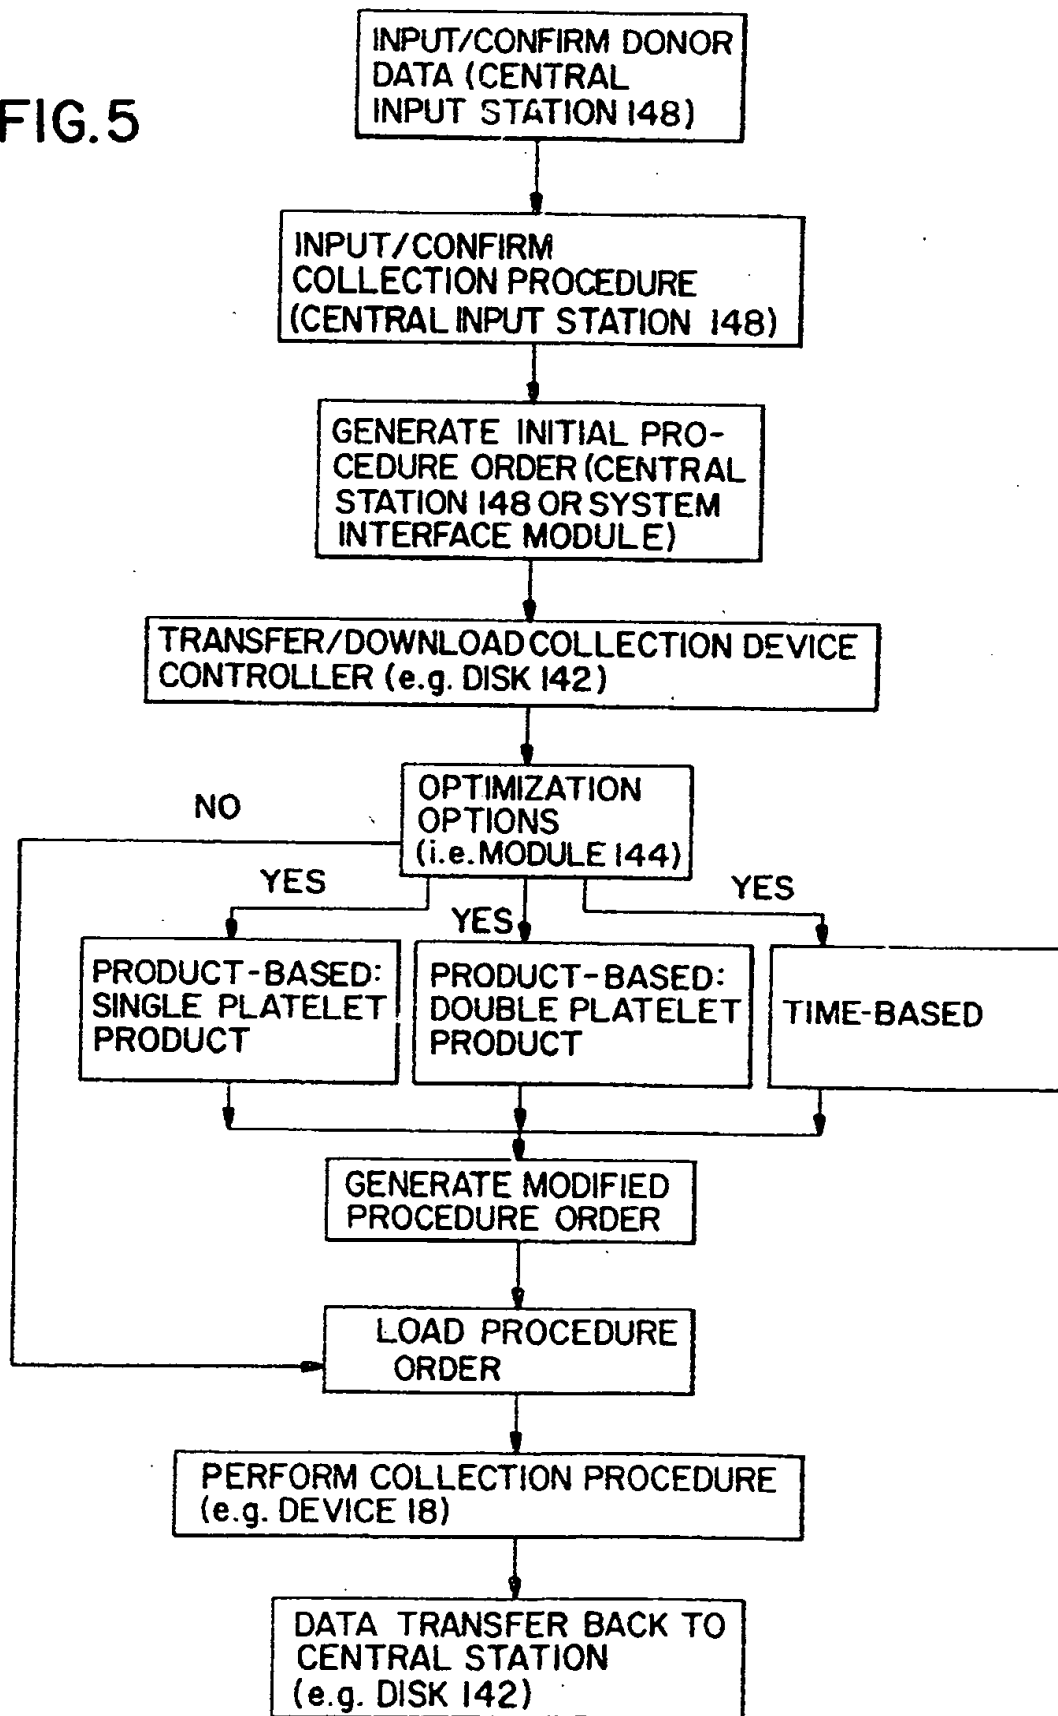

11 10 9 8 7 6 5 4 3 2 1


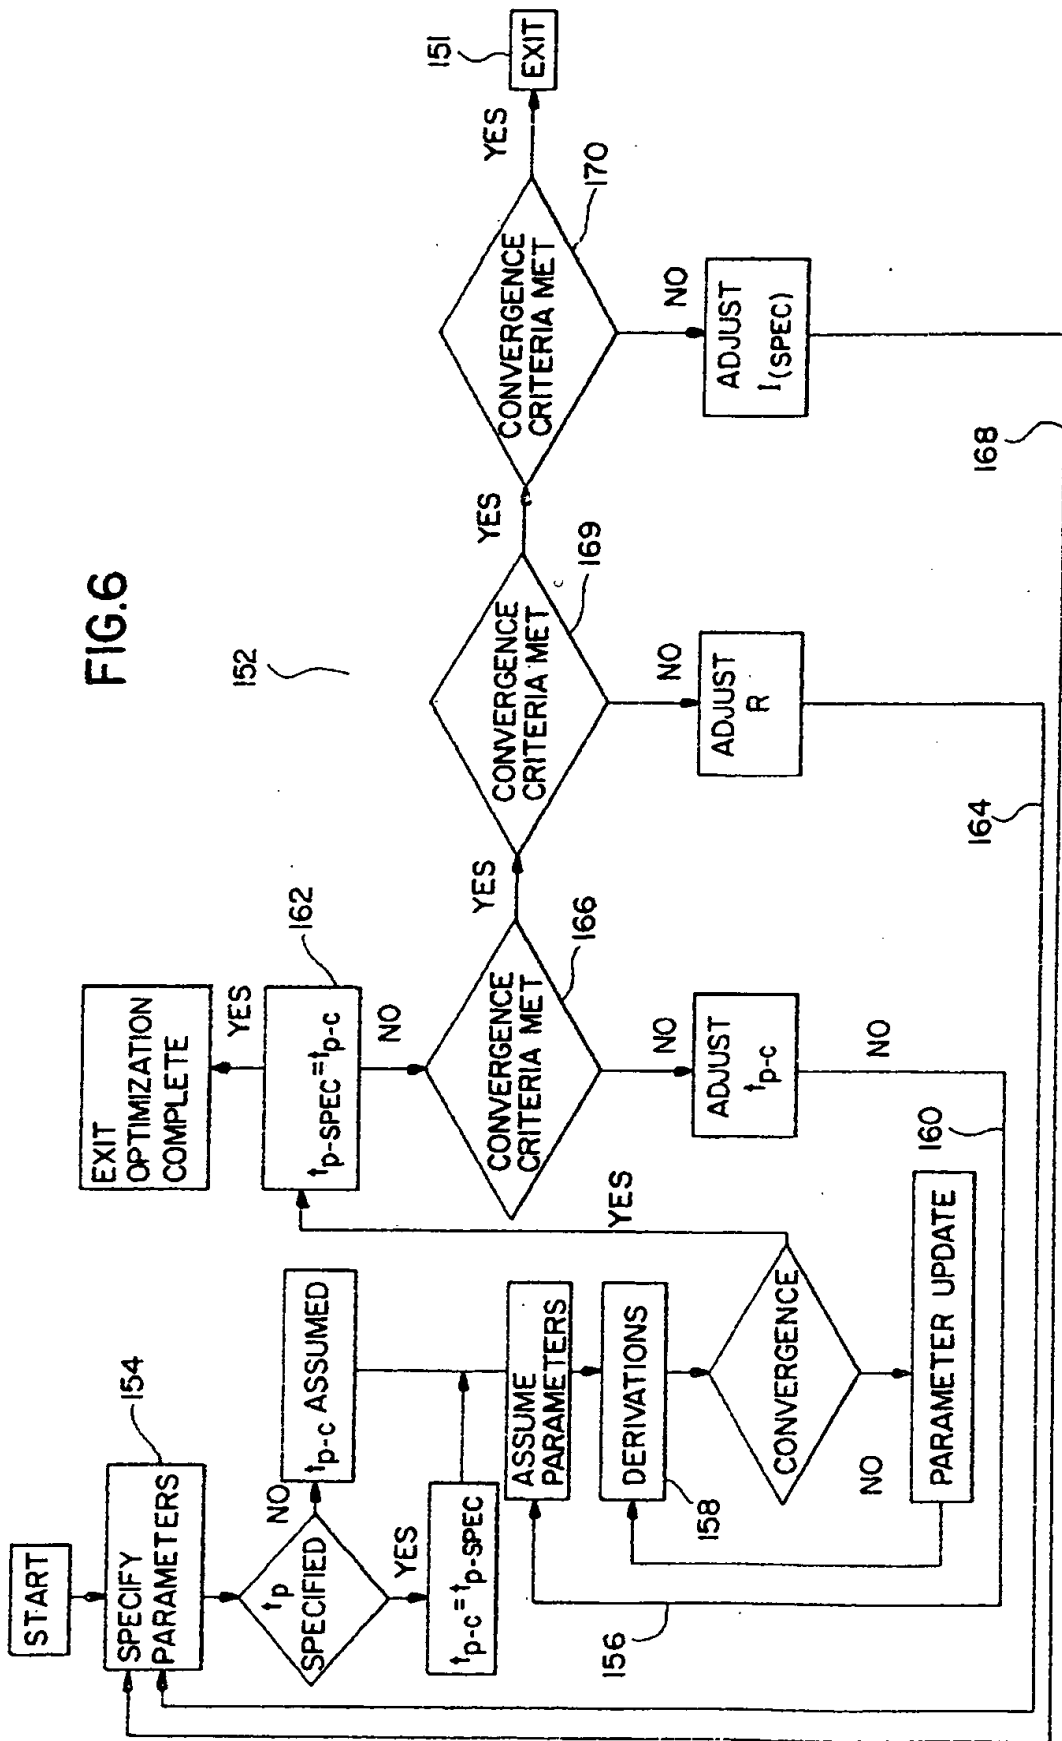


FIG. 7



9/9

FIG. 8

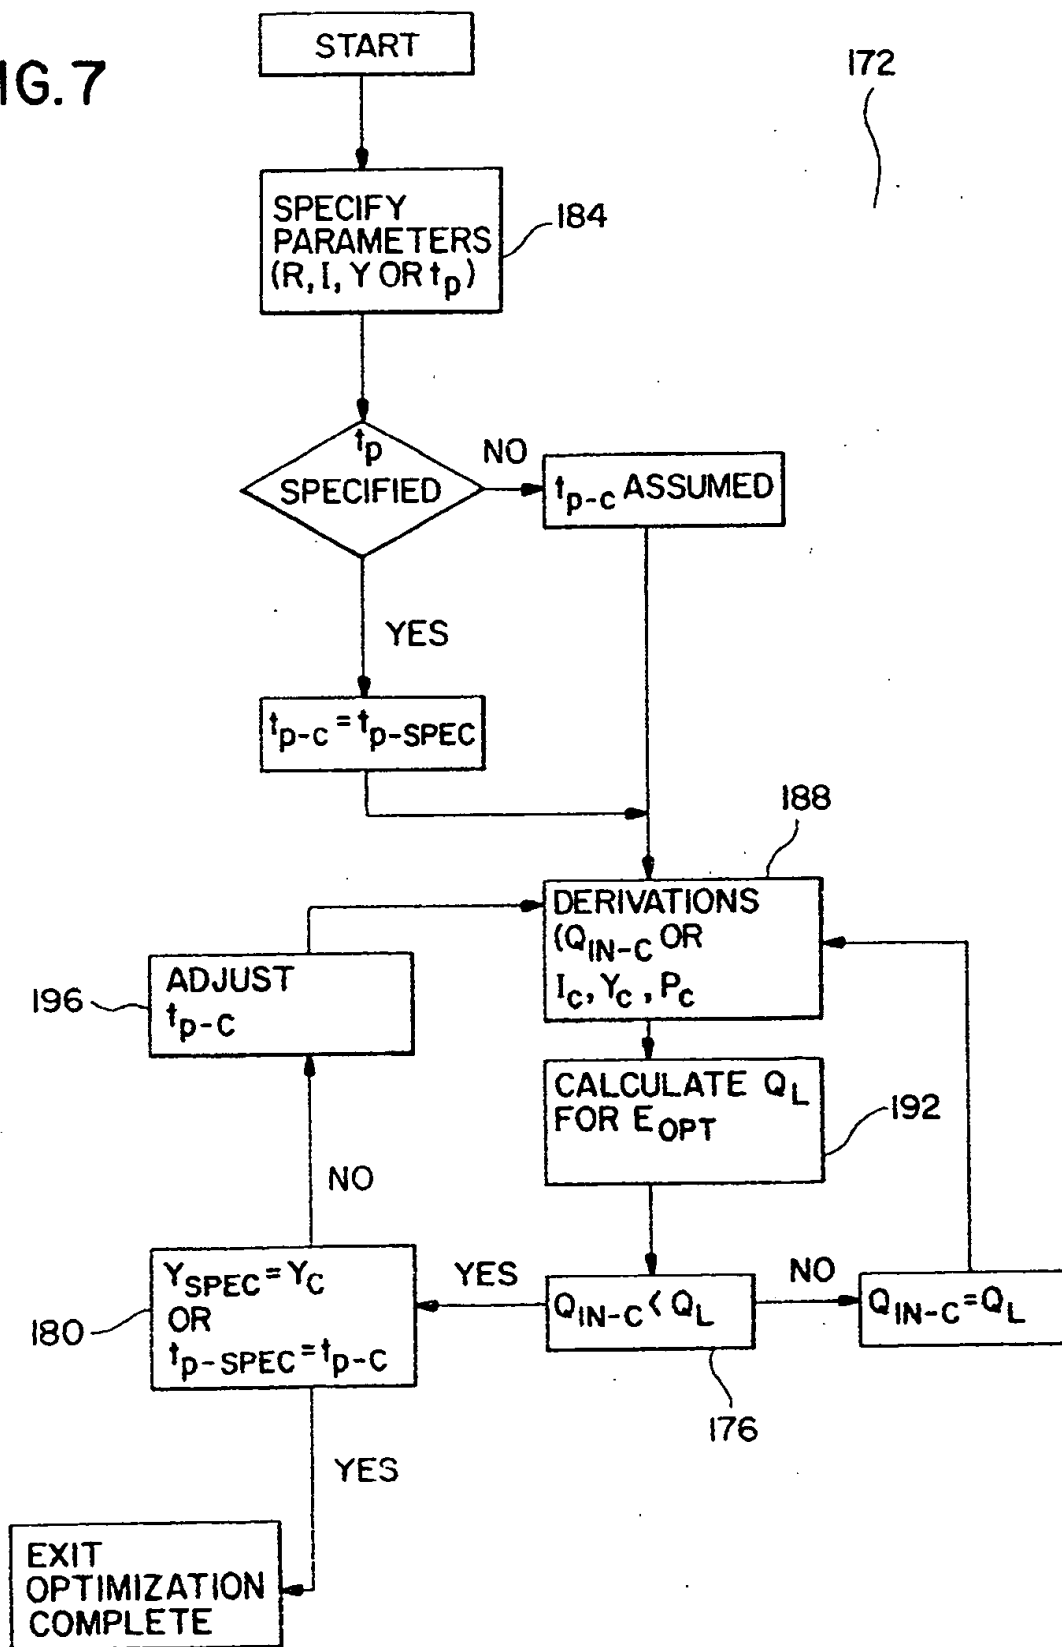